



File ..DATA\2021\20210317\1307\CPK2021-317-32429.D Tgt Mass (CHM):
 Injection Date : 17 Mar 21 8:38 pm +0800 Seq. Line : 142
 Sample Name : CPK2021-317-32429 Location : P1-D-03
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210317\1307\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210317\1307\1-POS-3MIN.M
 CAS NO. : 38183-03-8
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

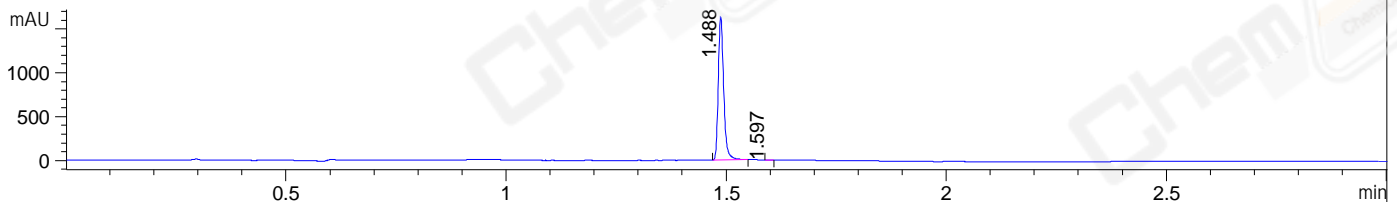


DAD1 C, Sig=254,4 Ref=off

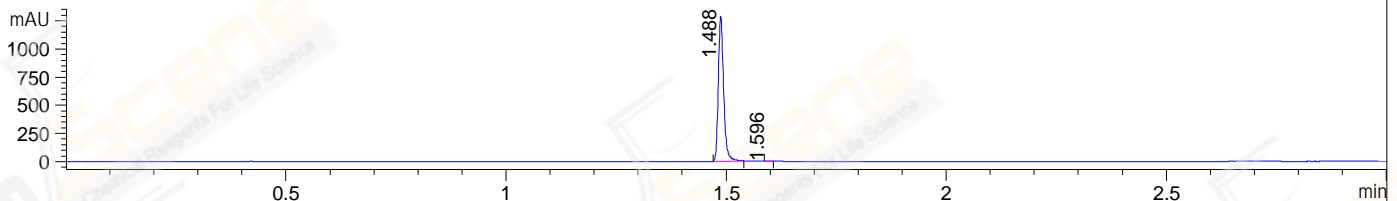

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

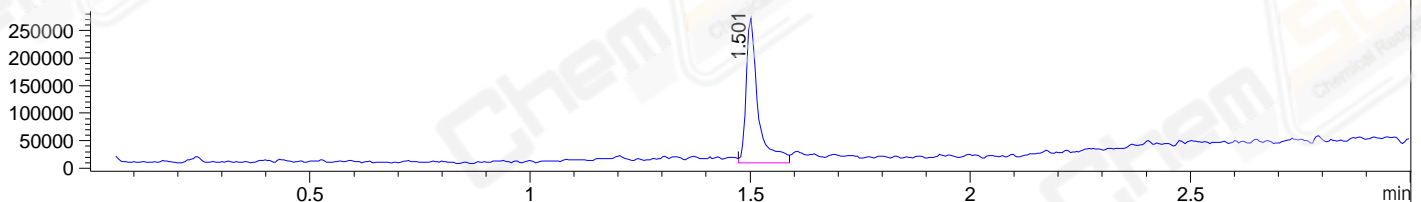

Ion 255, MSD1 255, Target Mass 254 +H Positive, EIC=254.7:255.7

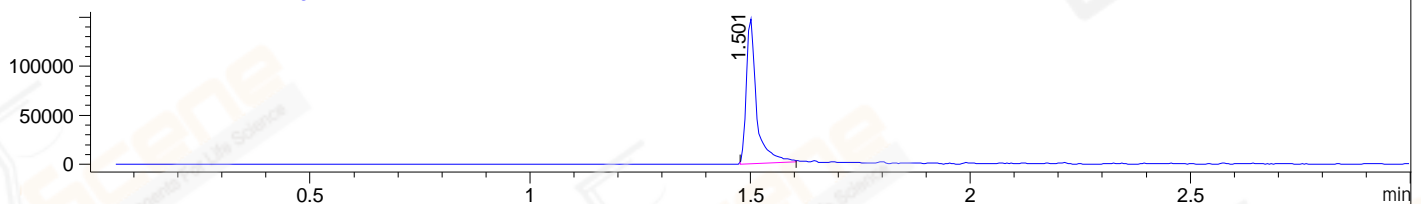

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.01	1407.89	1641.33	99.90	255
1.60	0.01	1.46	2.19	0.10	255

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.01	1084.19	1290.92	99.77	255
1.60	0.01	2.45	3.29	0.23	255

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.50	0.03	497798.31	263508.28	100.00	255

Ret. Time: 1.50

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

