



## Chromatogram and Results

### Injection Details

Injection Name:	CPK2021-419-33273	Run Time (min):	21.00
Vial Number:	GD1	Users:	ly
Injection Type:	Unknown	Injection Volume:	1.00
Calibration Level:		Channel:	UV_VIS_1
Instrument Method:	HM-414_13-H01P01(RP-HPLC)	Wavelength:	290
Processing Method:	3D Quantitative	Bandwidth:	4
CAS NO.:	1234015-54-3 A-RP-537	Dilution Factor:	1.0000
Injection Date/Time:	20/Apr/21 15:17	Sample Weight:	1.0000

chrom://hy442/ATA2/Instrument Data/202104/20210420.seq/836.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

### Chromatogram

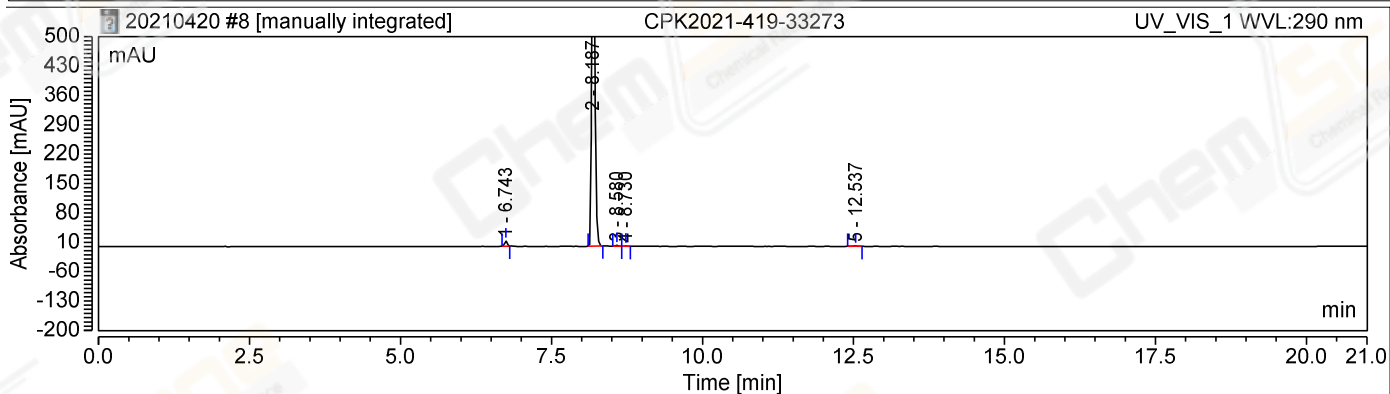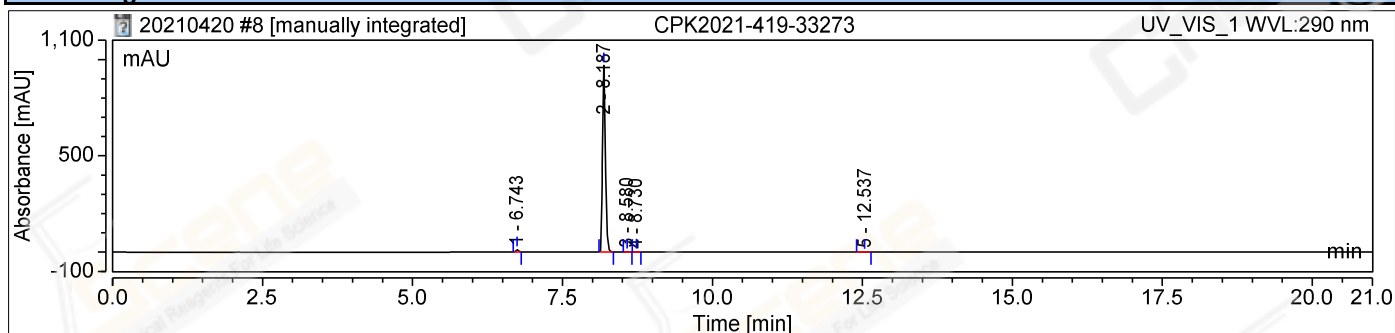

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Match	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		6.743	0.609	12.710	997	17.69	1.13	1.11
2		8.187	54.085	969.192	999	4.50	1.30	98.38
3		8.580	0.125	2.168	888	1.78	1.17	0.23
4		8.730	0.064	1.242	806	36.74	1.17	0.12
5		12.537	0.094	1.137	787	n.a.	0.94	0.17
Total:			54.977	986.449			60.71	5.72