



File ..1\DATA\2019\20190122\556\BIZ2019-122-WYQ2.D Tgt Mass (CHM):
Injection Date : 22 Jan 19 5:27 pm +0800 Seq. Line : 8
Sample Name : BIZ2019-122-WYQ2 Location : P2-E-06
Acq. Operator : LQ_1052 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190122\556\1-POS-3MIN-1.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190122\556\1-POS-3MIN-1.M
Catalog No : CS-0109 Batch#37026
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

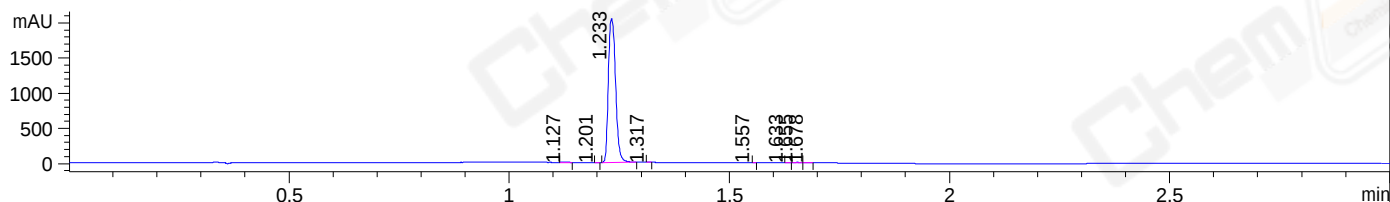


DAD1 C, Sig=254,4 Ref=off

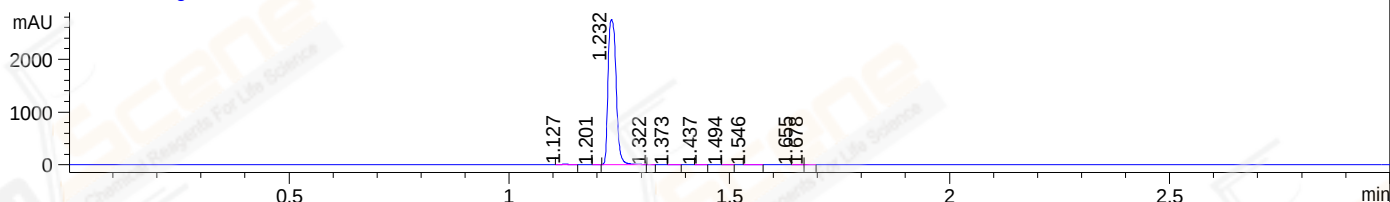

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

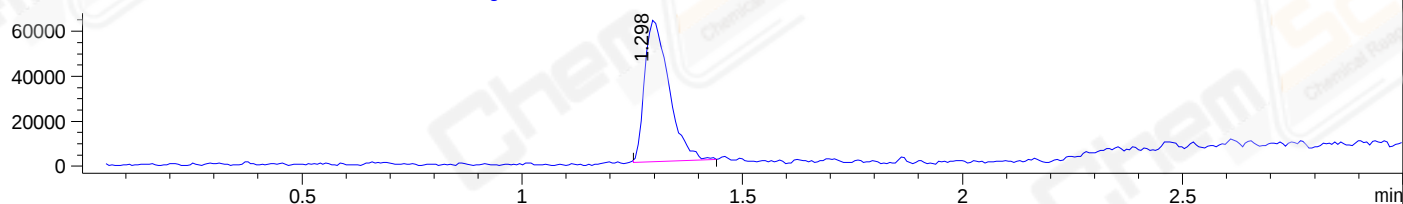

Ion 427.1, MSD1 427.1, Target Mass 426.1 +H Positive, EIC=426.8:427.8

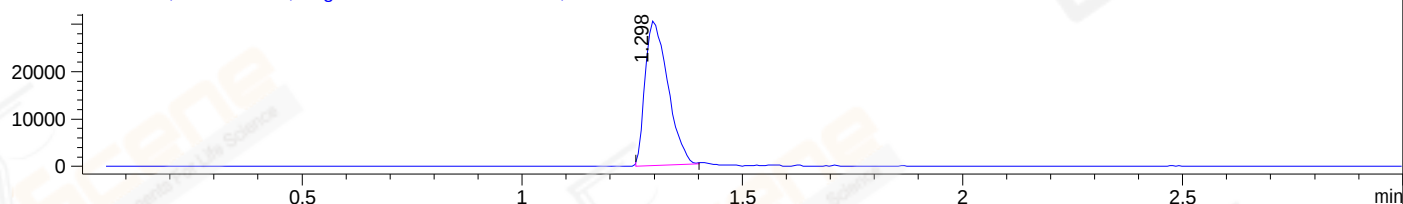

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.02	6.35	6.94	0.27	ND
1.20	0.01	0.51	1.20	0.02	ND
1.23	0.02	2330.00	2046.76	99.33	427
1.32	0.01	0.29	0.69	0.01	427
1.56	0.01	0.22	0.51	0.01	ND
1.63	0.01	0.77	1.22	0.03	ND
1.65	0.02	4.31	4.59	0.18	ND
1.68	0.01	3.30	3.75	0.14	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.02	11.62	12.09	0.33	ND
1.20	0.01	1.26	1.70	0.04	ND
1.23	0.02	3491.51	2752.77	99.20	427
1.32	0.01	0.61	0.85	0.02	427
1.37	0.02	0.85	0.77	0.02	427
1.44	0.02	1.75	1.66	0.05	ND

1.49	0.02	0.73	0.77	0.02	274
1.55	0.03	2.97	1.83	0.08	ND
1.65	0.02	5.69	5.55	0.16	ND
1.68	0.01	2.59	2.99	0.07	ND

Integration Results for MSD1 TIC, MS File

RetTime	Width	Area	Height	Area%	MS (+)
1.30	0.05	242202.83	63256.22	100.00	427

Ret. Time: 1.30

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

