



File ..1\DATA\2019\20190219\544\BIZ2019-218-WYQ2.D Tgt Mass (CHM):
Injection Date : 19 Feb 19 7:15 pm +0800 Seq. Line : 40
Sample Name : BIZ2019-218-WYQ2 Location : P1-B-09
Acq. Operator : LQ_1052 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190219\544\1-POS-3MIN-1.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190219\544\1-POS-3MIN-1.M
Catalog No : CS-4256 Batch#37564
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

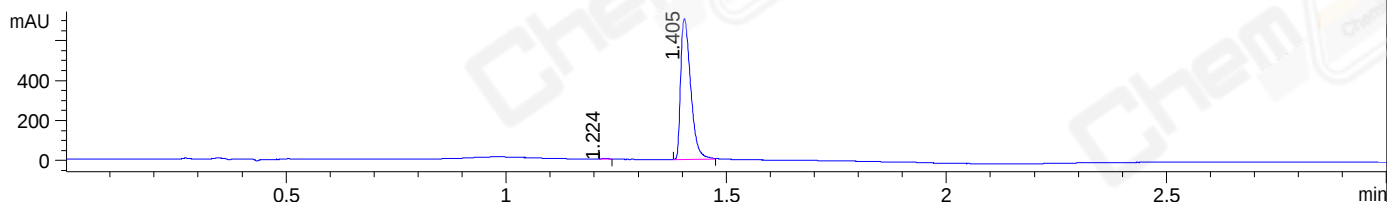


DAD1 C, Sig=254,4 Ref=off

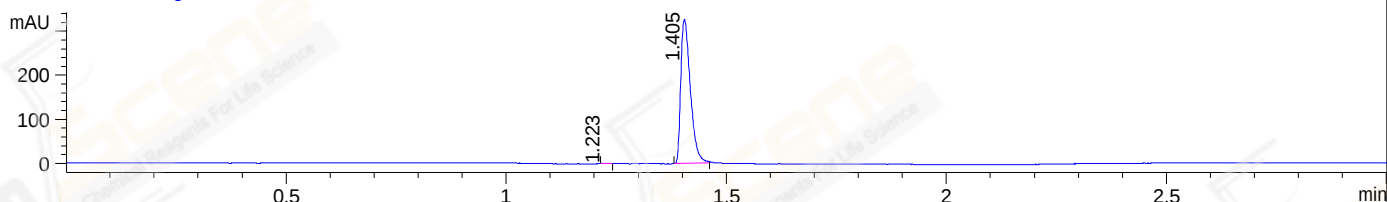

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

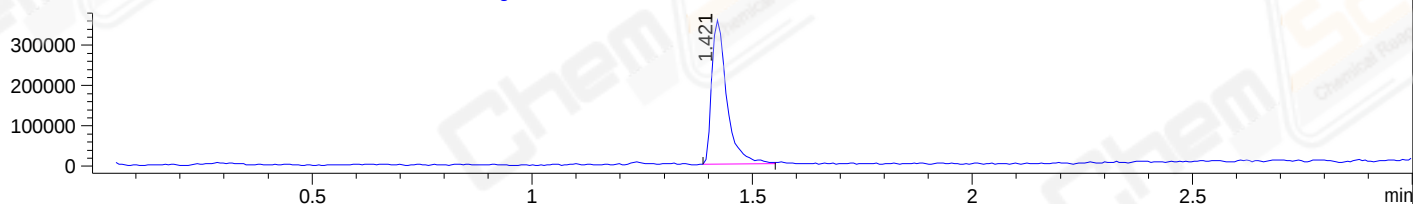

Ion 418.1, MSD1 418.1, Target Mass 417.1 +H Positive, EIC=417.8:418.8

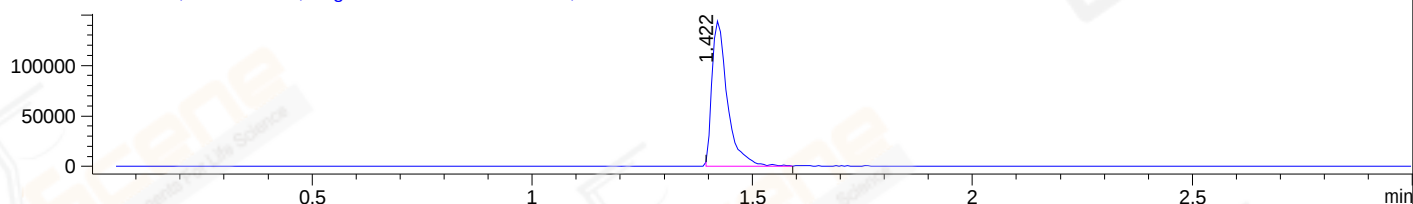

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	4.06	3.73	0.36	259
1.40	0.02	1112.97	704.63	99.64	418

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	0.52	0.50	0.10	259
1.40	0.02	494.64	327.09	99.90	418

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.42	0.04	855526.56	357499.91	100.00	418

Ret. Time: 1.42

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

