

File ..1\DATA\2019\20190410\559\BIZ2019-409-WYQ3.D Tgt Mass (CHM):

Injection Date : 10 Apr 19 2:34 pm +0800 Seq. Line : 69

Sample Name : BIZ2019-409-WYQ3 Location : P1-E-09

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190410\559\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190410\559\1-POS-3MIN-1.M

CAS NO. : 95058-81-4

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

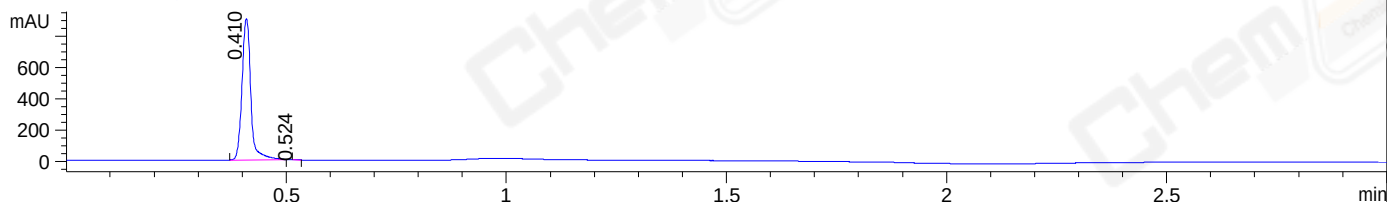


DAD1 C, Sig=254,4 Ref=off

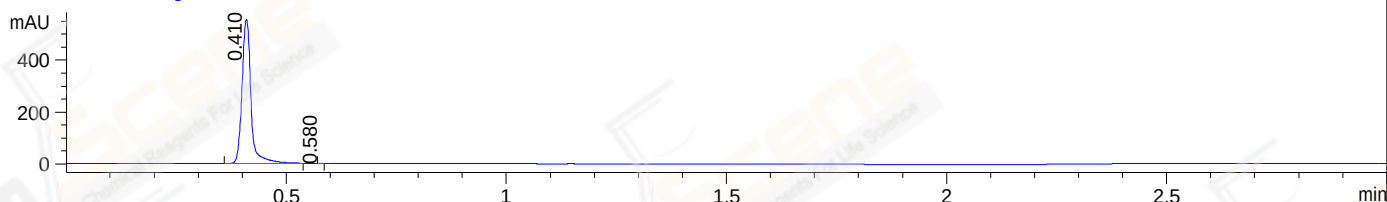

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

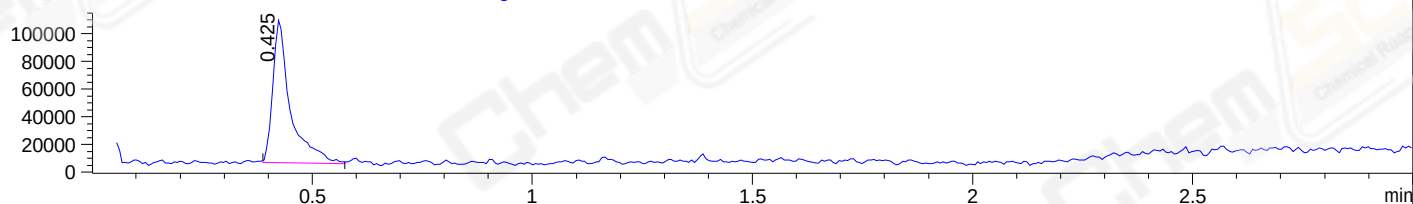

Ion 264, MSD1 264, Target Mass 263 +H Positive, EIC=263.7:264.7

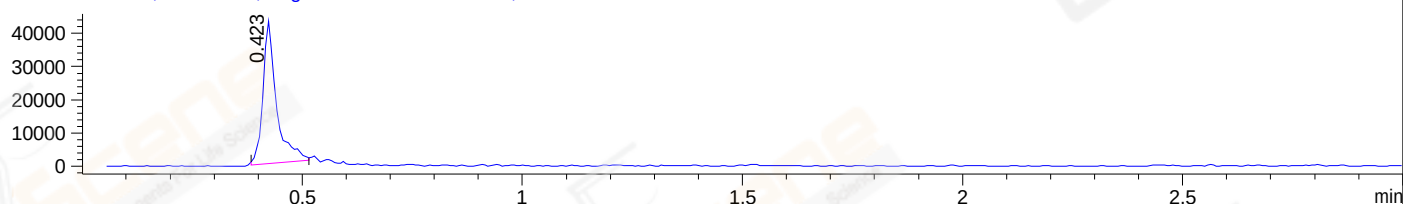

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
0.41	0.02	1254.89	903.46	99.92	527
0.52	0.01	1.03	1.33	0.08	527

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
0.41	0.02	788.01	556.13	99.99	527
0.58	0.01	0.05	0.09	0.01	157

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
0.42	0.04	287527.56	103857.08	100.00	527

Ret. Time: 0.42

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

