



File ..1\DATA\2019\20190520\583\BIZ2019-520-WYQ7.D Tgt Mass (CHM):
 Injection Date : 20 May 19 4:31 pm +0800 Seq. Line : 27
 Sample Name : BIZ2019-520-WYQ7 Location : P1-B-08
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190520\583\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190520\583\1-POS-3MIN.M
 Catalog No : CS-1526 Batch#41205
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-322
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

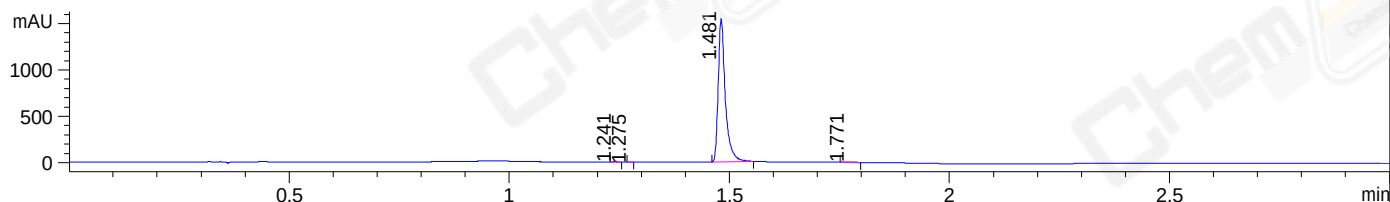


DAD1 C, Sig=254,4 Ref=off

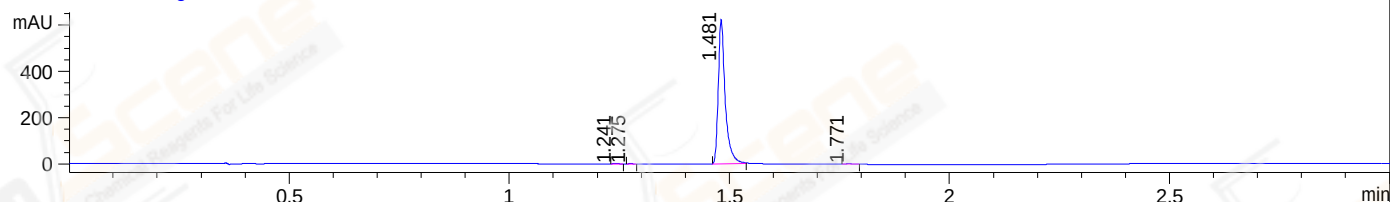

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

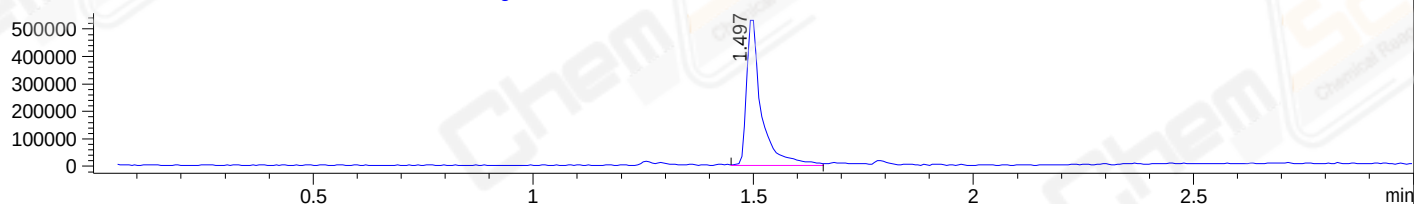

Ion 340.1, MSD1 340.1, Target Mass 339.1 +H Positive, EIC=339.8:340.8

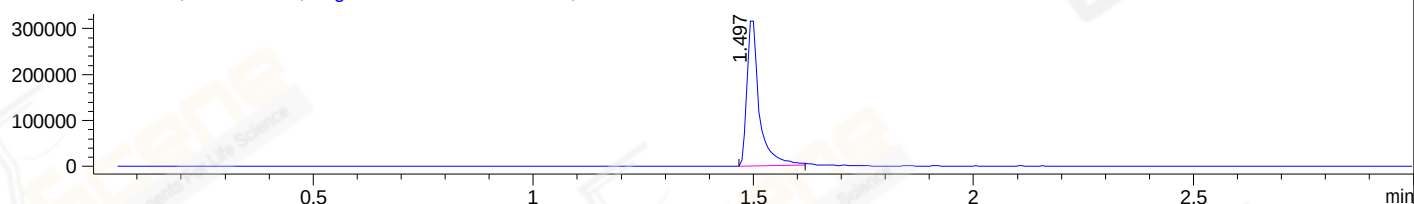

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.01	3.54	3.96	0.20	322
1.28	0.01	0.88	1.40	0.05	322
1.48	0.02	1748.94	1547.23	99.31	340
1.77	0.02	7.79	6.41	0.44	571

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.02	2.00	2.10	0.29	322
1.28	0.01	0.91	1.21	0.13	322
1.48	0.02	686.54	624.61	99.15	340
1.77	0.02	2.96	2.93	0.43	571

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.50	0.03	1232348.38	546714.38	100.00	340

Ret. Time: 1.50

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

