



File ..1\DATA\2019\20190430\564\BIZ2019-429-CXL6.D Tgt Mass (CHM):
Injection Date : 30 Apr 19 12:30 pm +0800 Seq. Line : 36
Sample Name : BIZ2019-429-CXL6 Location : P2-A-01
Acq. Operator : LQ_1052 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190430\564\1-POS-3MIN-1.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190430\564\1-POS-3MIN-1.M
CAS NO. : 1029044-16-3
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-322
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

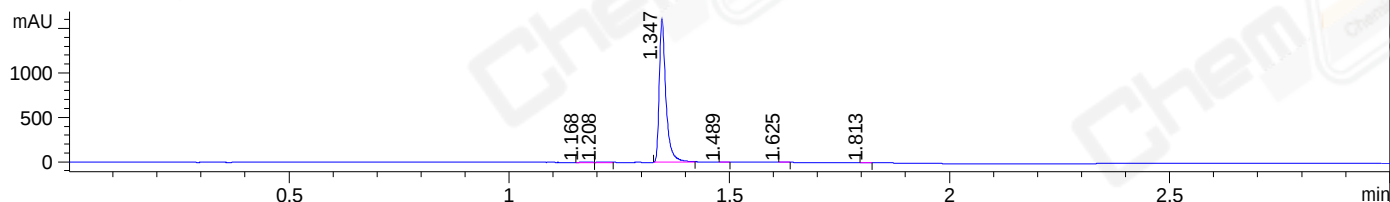


DAD1 C, Sig=254,4 Ref=off

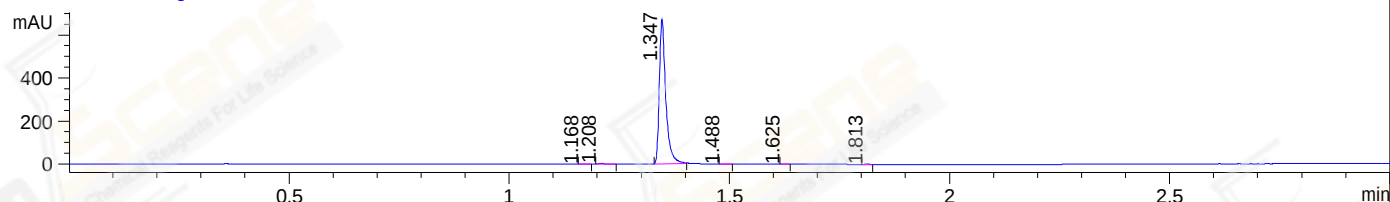

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

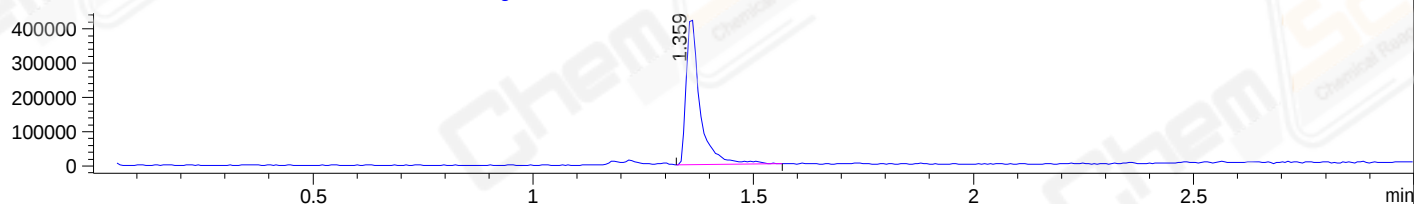

Ion 418.1, MSD1 418.1, Target Mass 417.1 +H Positive, EIC=417.8:418.8

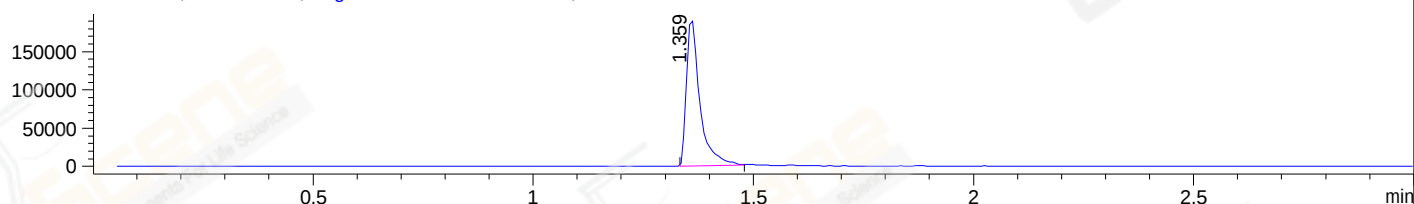

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	8.19	7.72	0.48	259
1.21	0.02	8.42	6.99	0.49	287
1.35	0.02	1689.24	1617.81	98.85	418
1.49	0.01	1.01	1.44	0.06	418
1.63	0.01	0.88	1.03	0.05	ND
1.81	0.02	1.14	1.03	0.07	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.01	1.01	1.18	0.15	259
1.21	0.02	3.25	2.75	0.47	287
1.35	0.02	687.40	673.20	99.13	418
1.49	0.01	1.05	1.25	0.15	418
1.63	0.01	0.39	0.48	0.06	ND
1.81	0.01	0.33	0.41	0.05	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.03	931970.19	432903.94	100.00	418

Ret. Time: 1.36

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

