



File ..1\DATA\2019\20190614\593\BIZ2019-613-CXL2.D Tgt Mass (CHM):
Injection Date : 14 Jun 19 1:49 pm +0800 Seq. Line : 64
Sample Name : BIZ2019-613-CXL2 Location : P2-F-05
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190614\593\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190614\593\1-POS-3MIN.M
Catalog No : CS-3285 Batch#42152
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

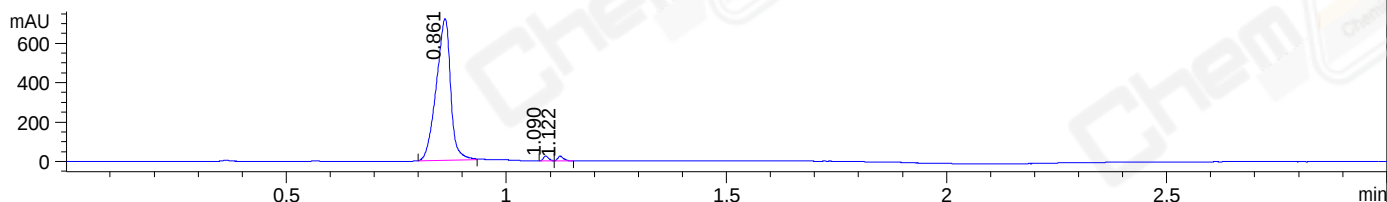


DAD1 C, Sig=254,4 Ref=off

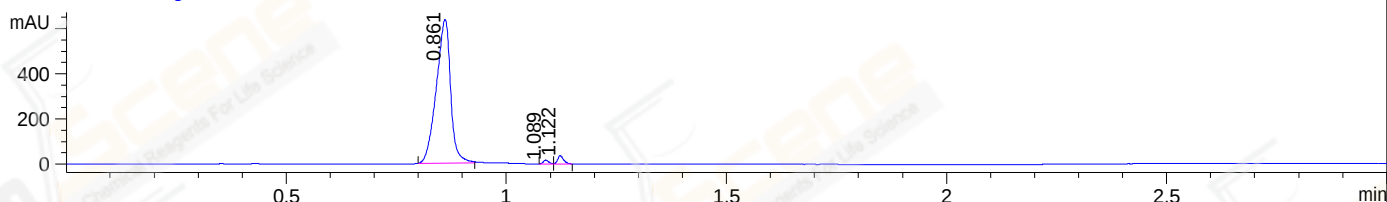

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

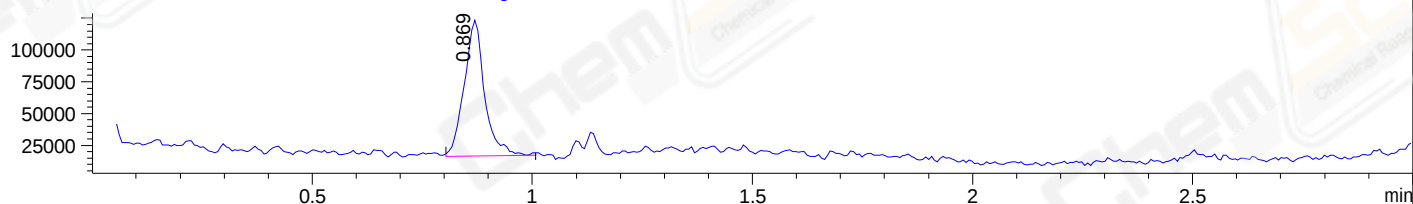

Ion 282.11, MSD1 282.11, Target Mass 281.11 +H Positive, EIC=281.81:282.81

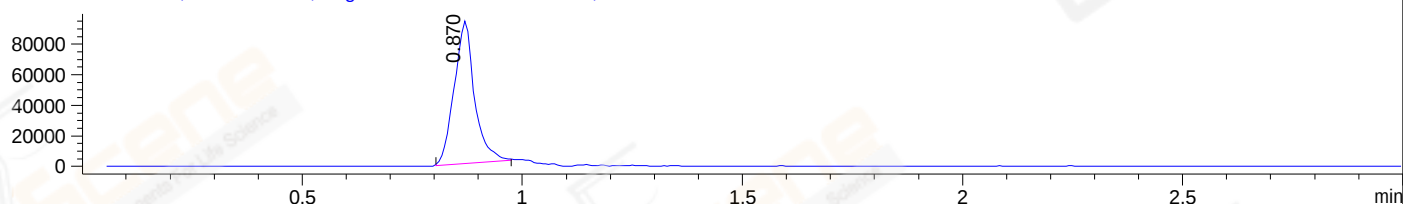

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.86	0.03	1633.24	720.52	97.35	282
1.09	0.01	21.35	25.80	1.27	157
1.12	0.01	23.15	24.76	1.38	157

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.86	0.03	1437.52	637.39	96.77	282
1.09	0.01	13.99	16.89	0.94	157
1.12	0.01	34.04	36.76	2.29	157

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.87	0.05	344177.09	107000.20	100.00	282

Ret. Time: 0.87

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

