



File ..1\DATA\2019\20190624\609\BIZ2019-621-WYQ4.D Tgt Mass (CHM):
Injection Date : 24 Jun 19 10:10 am +0800 Seq. Line : 16
Sample Name : BIZ2019-621-WYQ4 Location : P1-A-05
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190624\609\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190624\609\1-POS-3MIN.M
Catalog No : CS-0096560 Batch#42551
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

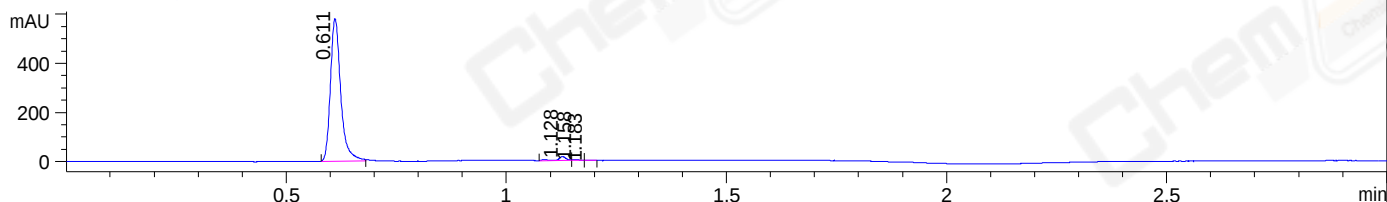


DAD1 C, Sig=254,4 Ref=off

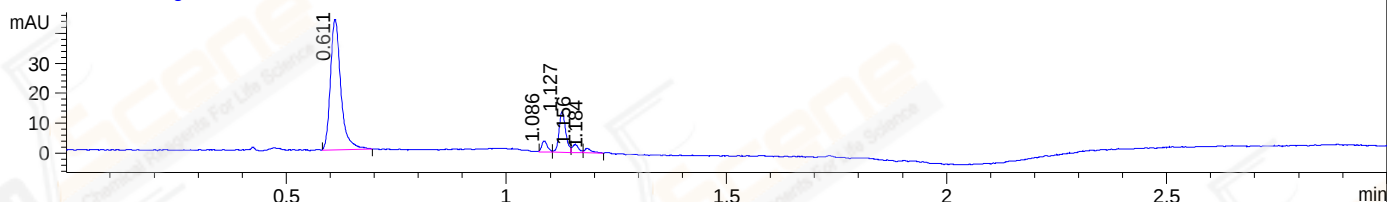

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

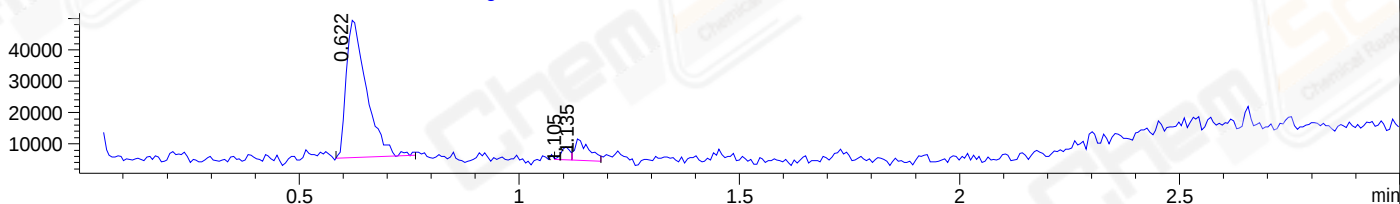

Ion 285, MSD1 285, Target Mass 284 +H Positive, EIC=284.7:285.7

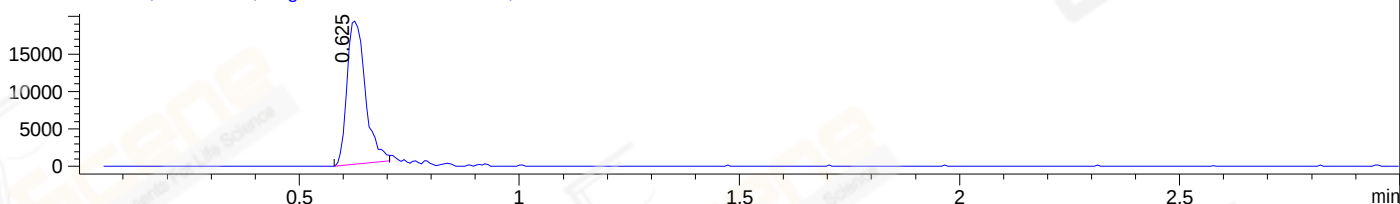

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.61	0.02	942.77	579.99	97.27	285
1.13	0.02	21.23	16.47	2.19	ND
1.16	0.02	4.17	4.55	0.43	ND
1.18	0.01	1.06	1.40	0.11	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.61	0.03	71.82	43.63	76.74	285
1.09	0.02	3.29	3.61	3.52	ND
1.13	0.02	14.14	13.58	15.11	ND
1.16	0.02	2.71	2.69	2.90	ND
1.18	0.02	1.62	1.49	1.73	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.61	0.03	71.82	43.63	76.74	285
1.09	0.02	3.29	3.61	3.52	ND
1.13	0.02	14.14	13.58	15.11	ND
1.16	0.02	2.71	2.69	2.90	ND
1.18	0.02	1.62	1.49	1.73	ND

0.62	0.04	140464.94	44326.00	87.37	285
1.11	0.02	5437.23	4081.02	3.38	ND
1.13	0.04	14868.37	7029.21	9.25	ND

Ret. Time: 0.62

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

