



File ..\DATA\2019\20190627\617\BIZ2019-626-CXL31.D Tgt Mass (CHM):
Injection Date : 27 Jun 19 2:21 pm +0800 Seq. Line : 64
Sample Name : BIZ2019-626-CXL31 Location : P1-A-05
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190627\617\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190627\617\1-POS-3MIN.M
Catalog No : CS-0150 Batch#42715
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

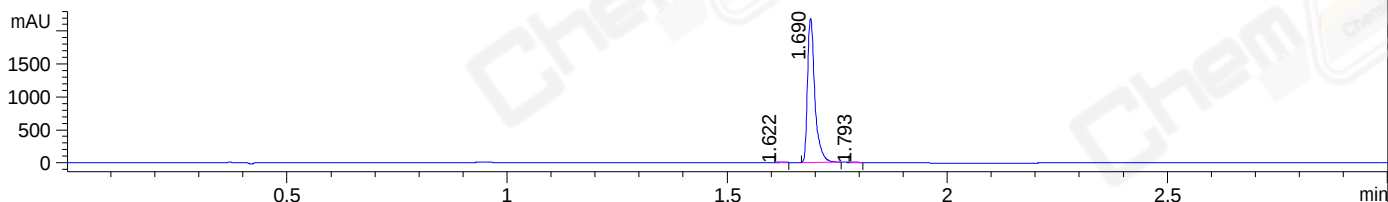


DAD1 C, Sig=254,4 Ref=off

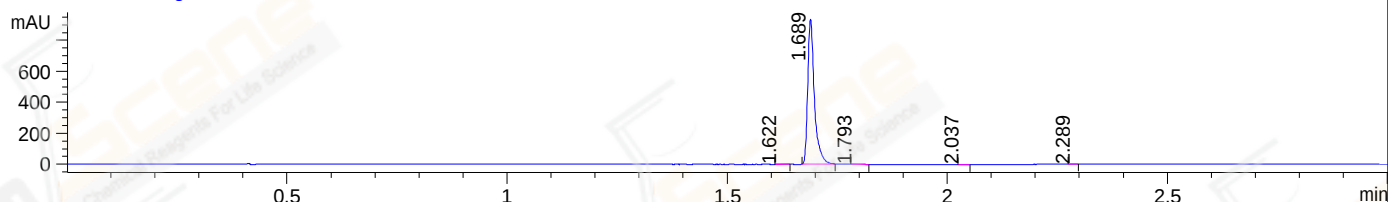

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

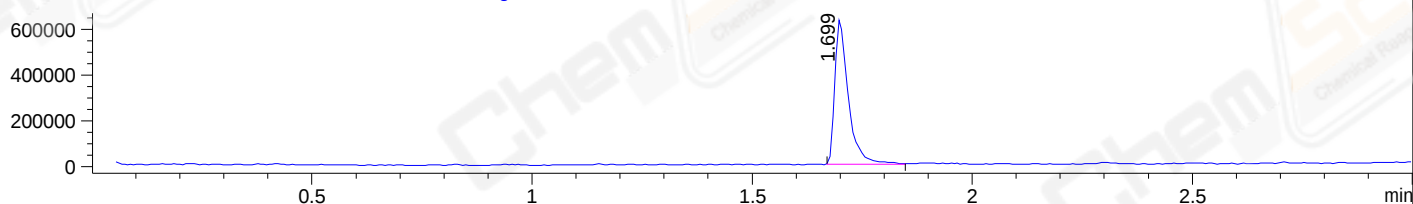

Ion 308.12, MSD1 308.12, Target Mass 307.12 +H Positive, EIC=307.82:308.82

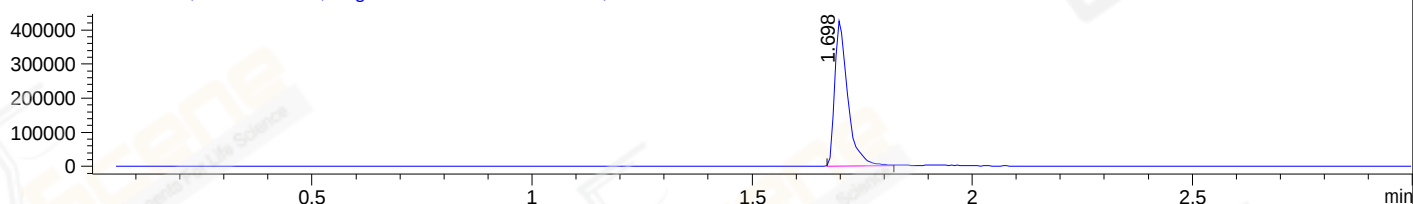

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.62	0.02	1.35	1.49	0.05	ND
1.69	0.02	2536.84	2186.04	99.86	308
1.79	0.02	2.17	2.25	0.09	308

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.62	0.02	0.78	0.74	0.08	ND
1.69	0.02	989.20	936.42	99.62	308
1.79	0.02	1.55	1.40	0.16	308
2.04	0.01	0.90	1.07	0.09	308
2.29	0.01	0.53	0.69	0.05	473

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.70	0.03	1370548.50	638524.63	100.00	308

Ret. Time: 1.70

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

