



File ..MS03\Data\20190716\20190716\DJL6871-029-4.D Tgt Mass (CHM):
Injection Date : 16 Jul 19 10:53 am +0800 Seq. Line : 24
Sample Name : DJL6871-029-4 Location : P1-C-01
Acq. Operator : SYSTEM Inj : 1
Spec. Reported : MS Integration Inj Volume : 2 ul
Acq. Method : D:\LCMS03\Data\20190716\20190716\1-POS-3MIN.M
Analysis Method : D:\LCMS03\Data\20190716\20190716\1-POS-3MIN.M
Catalog No : CS-0093244 Batch# 43590
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-446
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

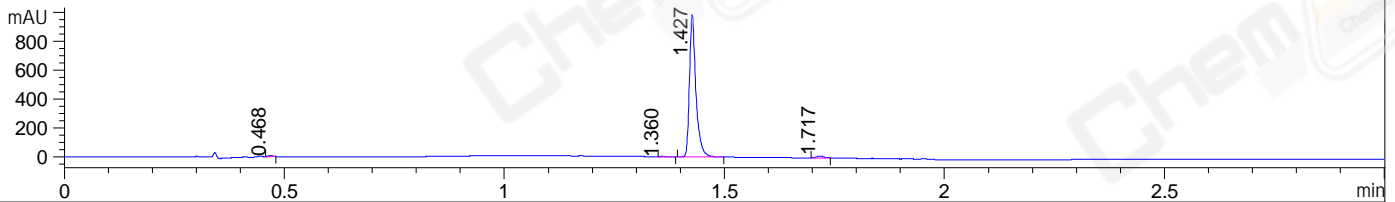


ELS1 A, ELSD Signal

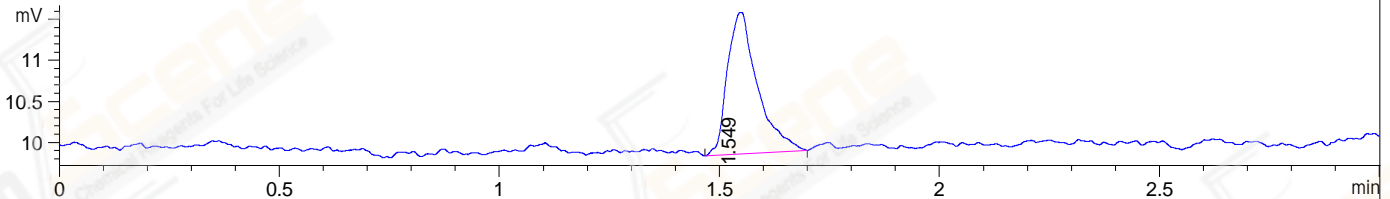

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

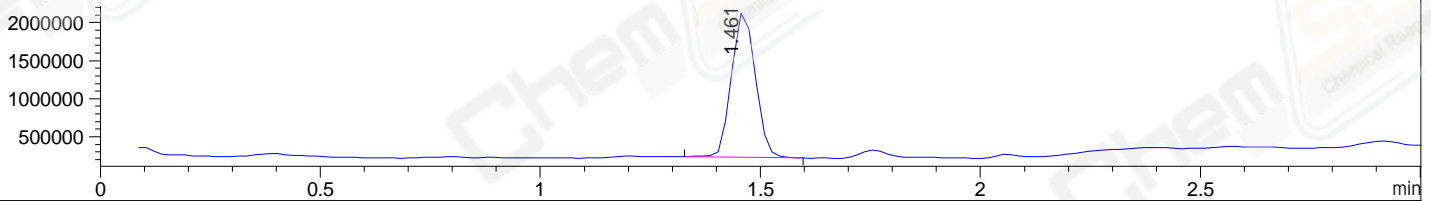

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

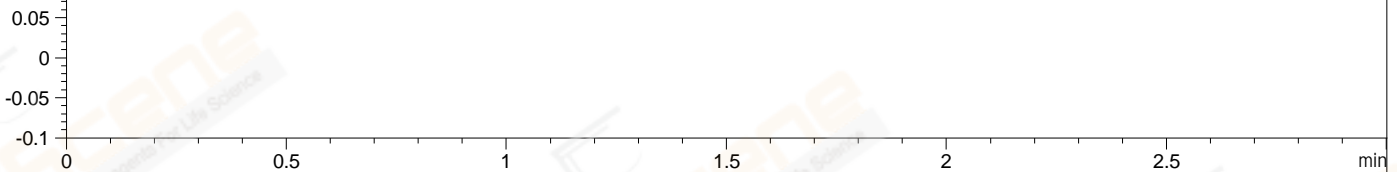

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.47	0.01	5.37	8.77	0.53	145
1.36	0.01	1.05	1.21	0.10	145
1.43	0.01	999.08	981.64	98.02	764
1.72	0.02	13.76	12.00	1.35	114


Integration Results for ELS1 A, ELSD Signal

RetTim	Width	Area	Height	Area%	MS (+)
1.55	0.07	8.25	1.73	100.00	764

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.46	0.06	7121339.50	1919233.38	100.00	764

Ret. Time: 1.46 <<<< POSITIVE SPECTRA >>>>

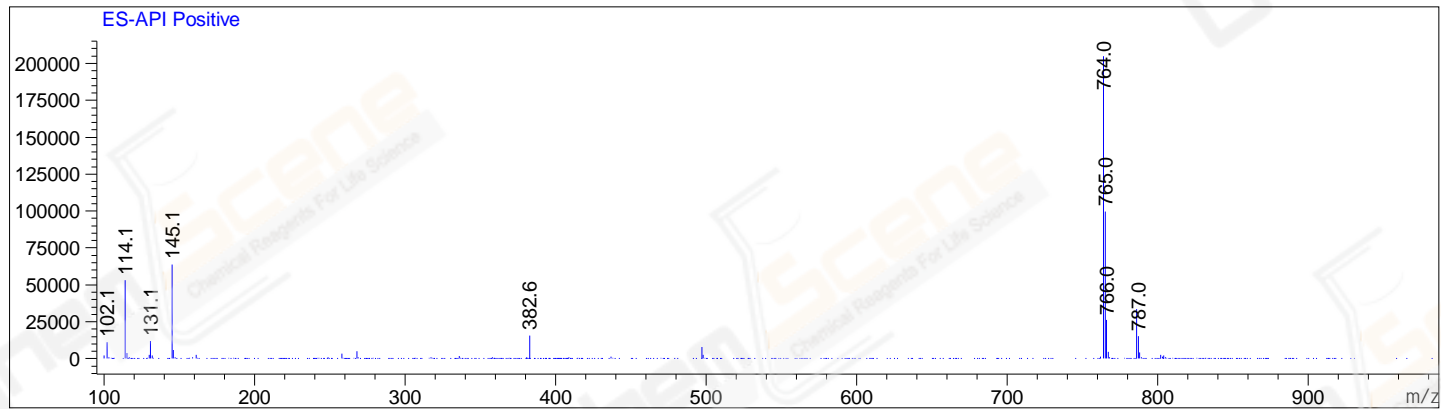

*** End of Report ***