



File ..S03\Data\20190801\20190801\SX7041-001-1_1.D Tgt Mass (CHM):
Injection Date : 1 Aug 19 2:19 pm +0800 Seq. Line : 54
Sample Name : SX7041-001-1_1 Location : P1-D-11
Acq. Operator : SYSTEM Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\LCMS03\Data\20190801\20190801\1-POS-3MIN.M
Analysis Method : D:\LCMS03\Data\20190801\20190801\1-POS-3MIN.M
Catalog No : CS-1285 Batch#44005
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-446
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

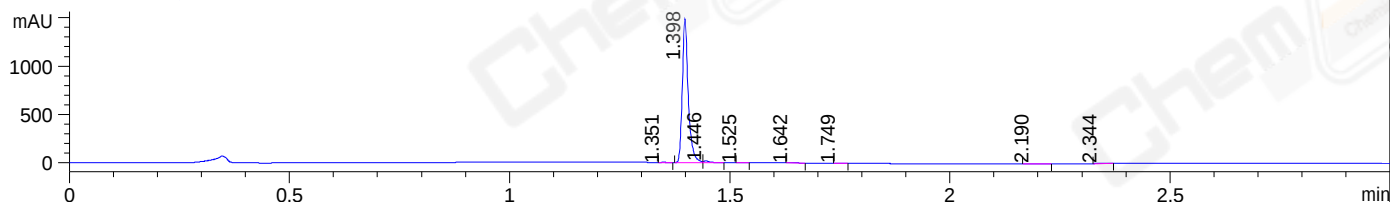


ELS1 A, ELSD Signal

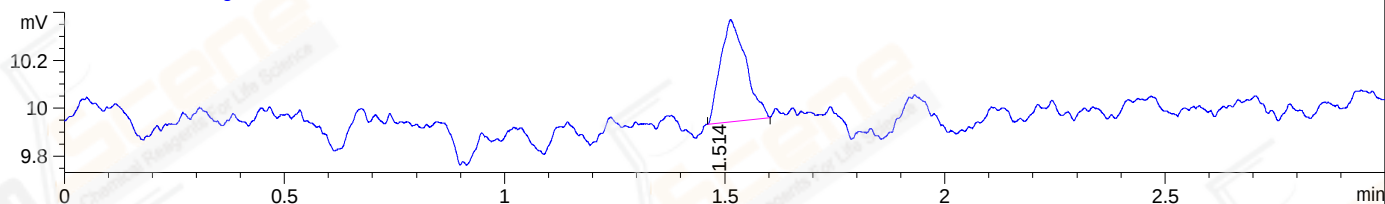

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

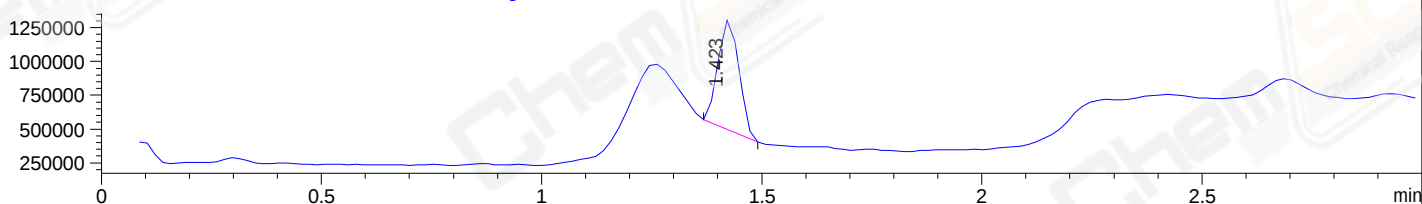

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

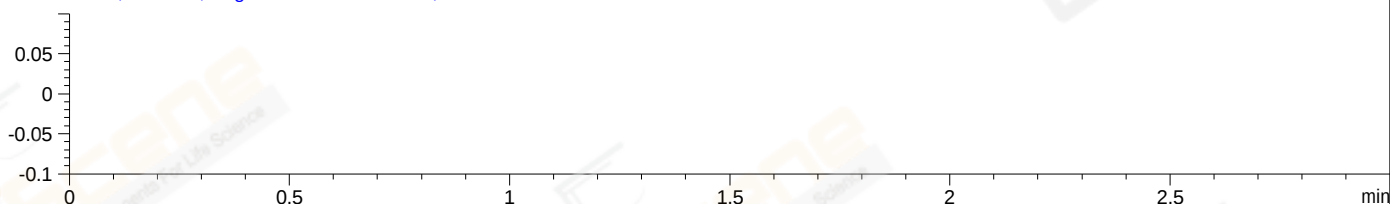

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.01	1.07	1.36	0.08	145
1.40	0.02	1397.47	1495.66	98.12	349
1.45	0.02	16.32	17.15	1.15	349
1.53	0.01	0.65	0.88	0.05	145
1.64	0.01	2.29	2.45	0.16	145
1.75	0.02	1.10	1.19	0.08	114
2.19	0.03	3.99	2.62	0.28	114
2.34	0.02	1.32	0.98	0.09	338

Integration Results for ELS1 A, ELSD Signal

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.07	1.73	0.43	100.00	145


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
--------	-------	------	--------	-------	--------

1.42	0.05	2674017.50	814079.50	100.00	349
------	------	------------	-----------	--------	-----

Ret. Time: 1.42

<<<< POSITIVE SPECTRA >>>>

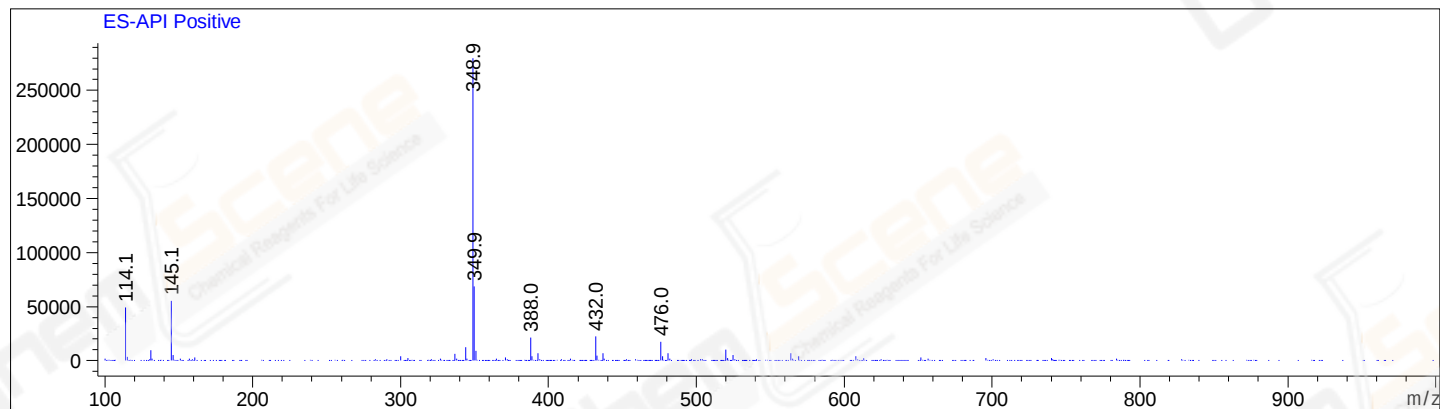

*** End of Report ***