



File ..1\DATA\2019\20190819\694\BIZ2019-816-CXL4.D Tgt Mass (CHM):
Injection Date : 19 Aug 19 10:58 am +0800 Seq. Line : 13
Sample Name : BIZ2019-816-CXL4 Location : P1-A-04
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 uL
Acq. Method : D:\Chem32\1\data\2019\20190819\694\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190819\694\1-POS-3MIN.M
Catalog No : CS-3521 Batch# 44407
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

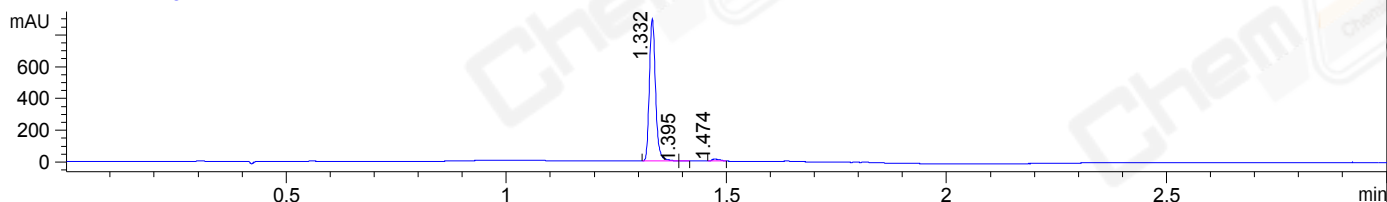


DAD1 C, Sig=254,4 Ref=off

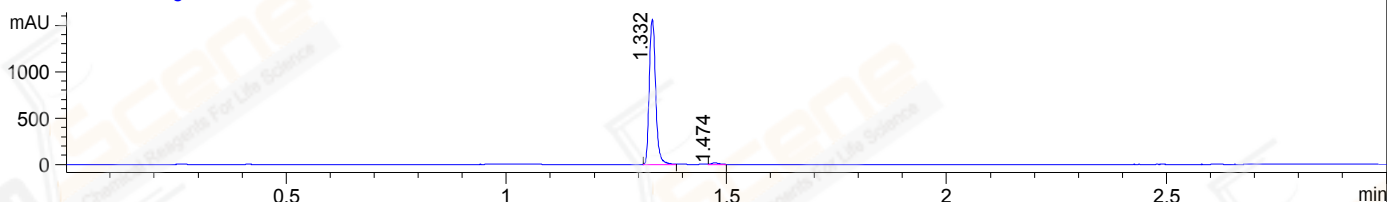

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

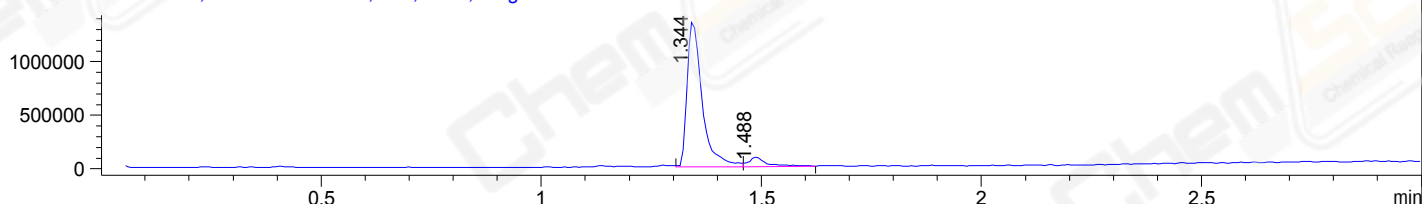

Ion 335.1, MSD1 335.1, Target Mass 334.1 +H Positive, EIC=334.8:335.8

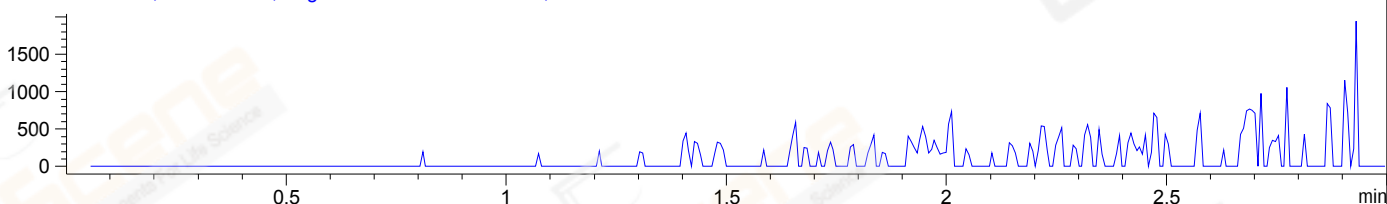

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.33	0.02	869.75	897.33	98.26	299
1.40	0.01	1.08	1.35	0.12	299
1.47	0.02	14.36	12.96	1.62	375

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.33	0.02	1572.18	1564.40	98.78	299
1.47	0.01	19.37	19.33	1.22	375

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.34	0.04	3228659.00	1363872.88	92.53	299
1.49	0.04	260595.47	88811.17	7.47	375

Ret. Time: 1.34

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.49

ES-API Positive

