



File ..1\DATA\2019\20190917\719\BIZ2019-912-WSD5.D Tgt Mass (CHM):
Injection Date : 17 Sep 19 11:08 am +0800 Seq. Line : 24
Sample Name : BIZ2019-912-WSD5 Location : P1-B-08
Acq. Operator : bgd_1571 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.7 ul
Acq. Method : D:\Chem32\1\data\2019\20190917\719\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190917\719\1-POS-3MIN.M
Catalog No : CS-0864 Batch#45596
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

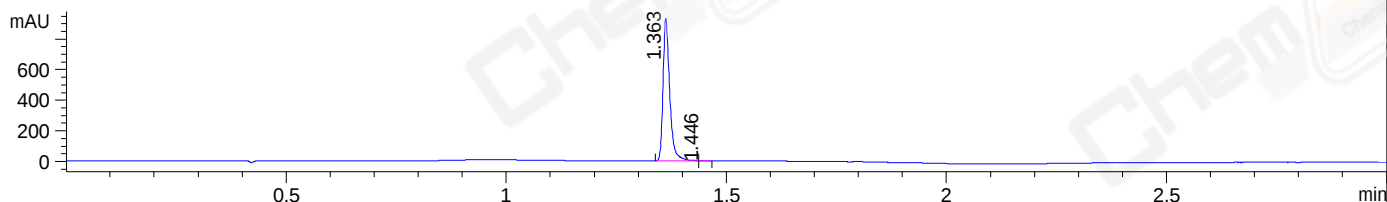


DAD1 C, Sig=254,4 Ref=off

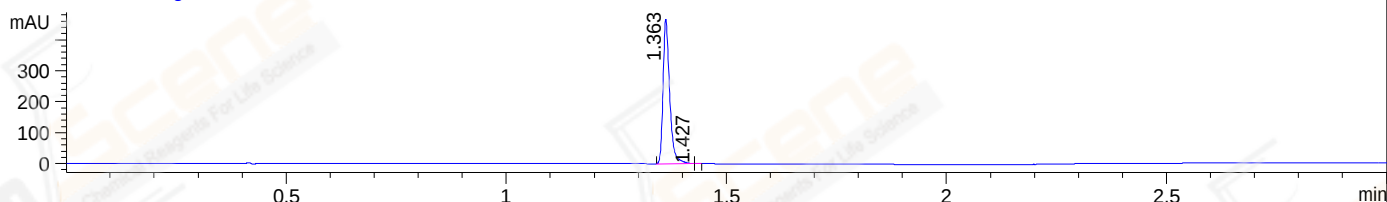

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

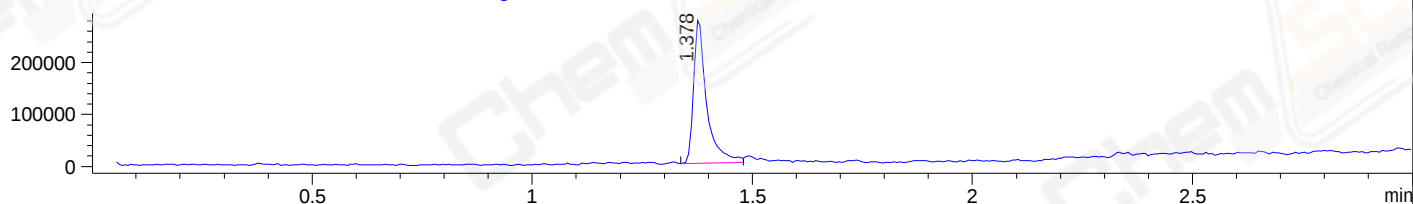

Ion 307.16, MSD1 307.16, Target Mass 306.16 +H Positive, EIC=306.86:307.86

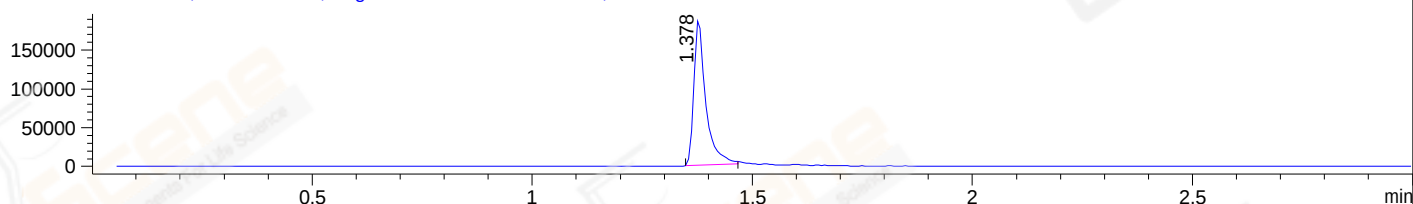

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	977.86	931.26	99.88	307
1.45	0.02	1.15	0.98	0.12	307

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	487.72	467.53	99.93	307
1.43	0.01	0.34	0.54	0.07	307

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	574353.00	282869.53	100.00	307

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

