



File ..DATA\2019\20190925\720\BIZ2019-924-SCH11.D Tgt Mass (CHM):
Injection Date : 25 Sep 19 4:18 pm +0800 Seq. Line : 100
Sample Name : BIZ2019-924-SCH11 Location : P1-C-04
Acq. Operator : bgd_1571 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.5 ul
Acq. Method : D:\Chem32\1\data\2019\20190925\720\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190925\720\1-POS-3MIN.M
Catalog No : CS-6764 Batch#46099
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

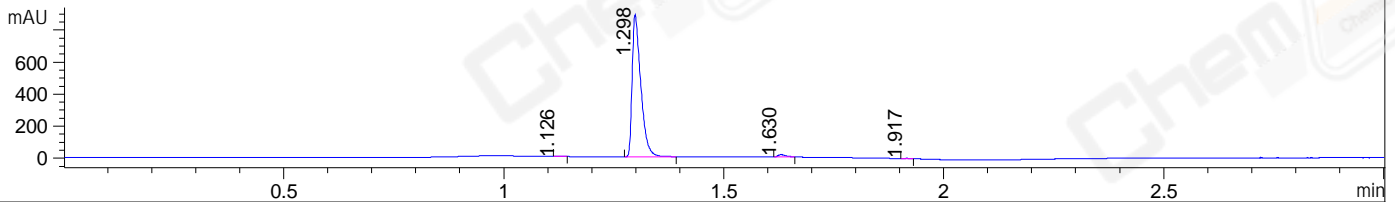


DAD1 C, Sig=254,4 Ref=off

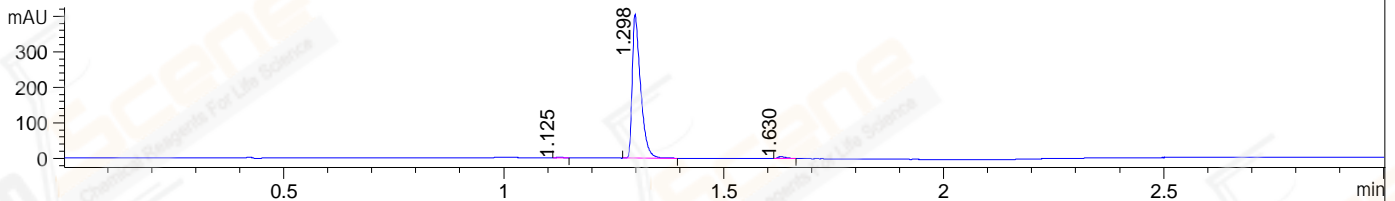

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

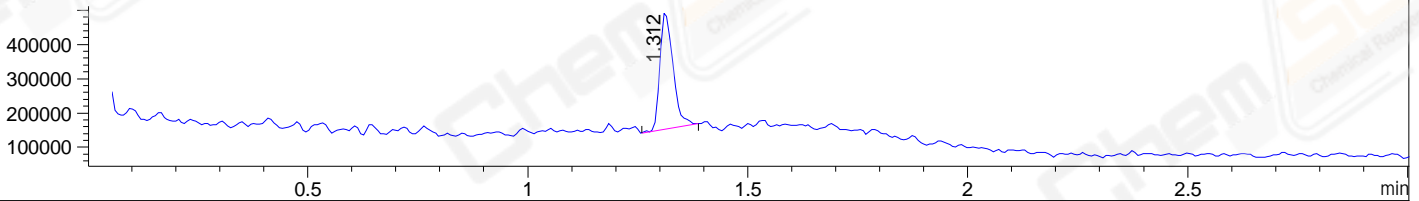

Ion 367.17, MSD1 367.17, Target Mass 366.17 +H Positive, EIC=366.87:367.87

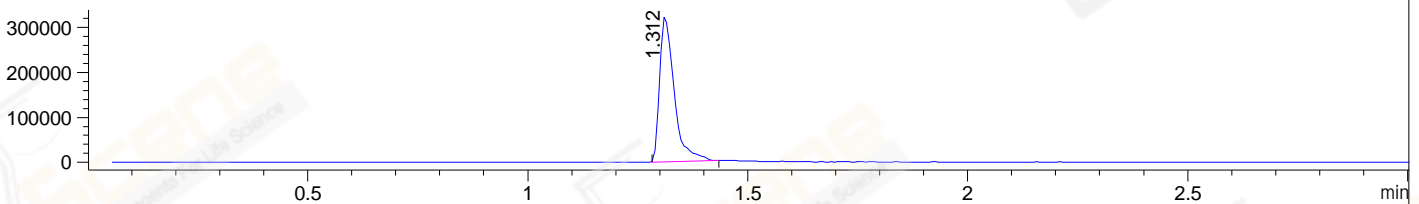

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.02	3.62	3.44	0.29	230
1.30	0.02	1208.01	888.57	98.17	367
1.63	0.02	17.03	14.98	1.38	230
1.92	0.02	1.90	2.02	0.15	230

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.02	1.84	1.55	0.34	230
1.30	0.02	532.28	404.90	98.52	367
1.63	0.02	6.15	5.04	1.14	230

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.31	0.03	707750.25	346985.53	100.00	367

Ret. Time: 1.31

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

