



File ..1\DATA\2019\20190926\720\BIZ2019-925-CXL3.D Tgt Mass (CHM):  
 Injection Date : 26 Sep 19 11:58 am +0800 Seq. Line : 34  
 Sample Name : BIZ2019-925-CXL3 Location : P1-B-08  
 Acq. Operator : bgd\_1571 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2019\20190926\720\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190926\720\1-POS-3MIN.M  
 Catalog No : CS-1117 Batch#46175  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

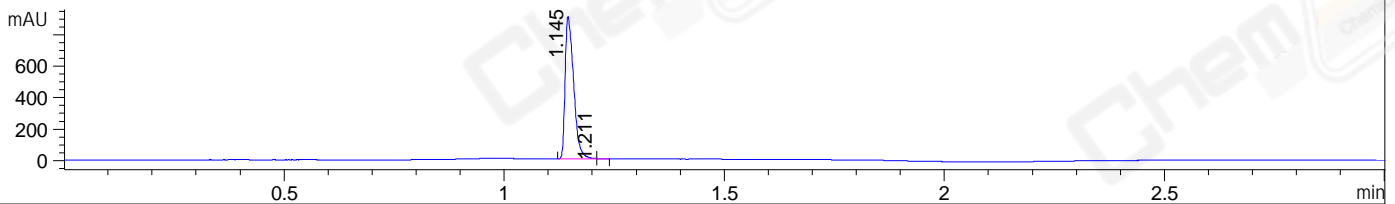


DAD1 C, Sig=254,4 Ref=off

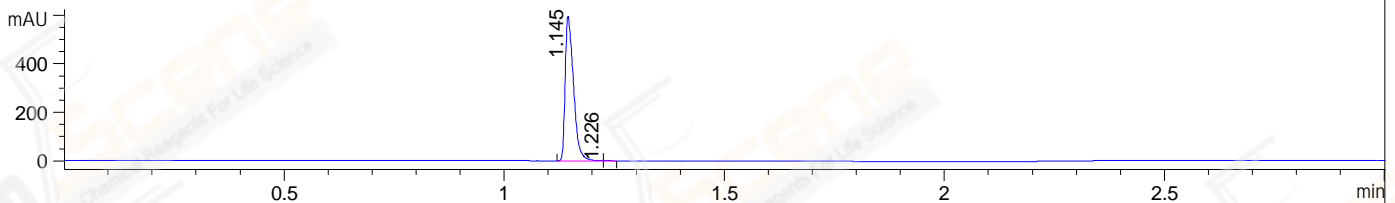

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

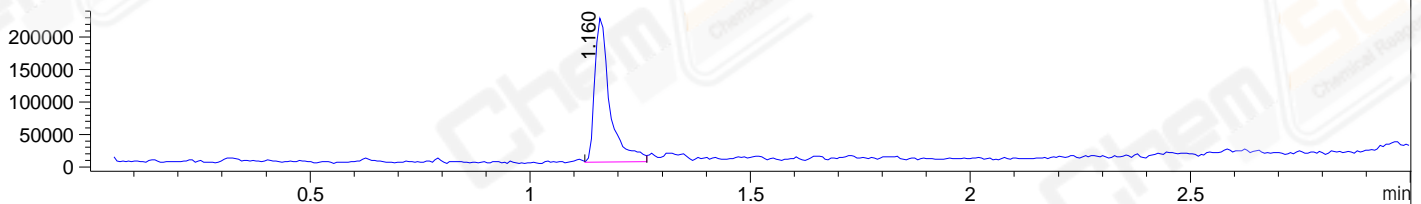

Ion 376.08, MSD1 376.08, Target Mass 375.08 +H Positive, EIC=375.78:376.78

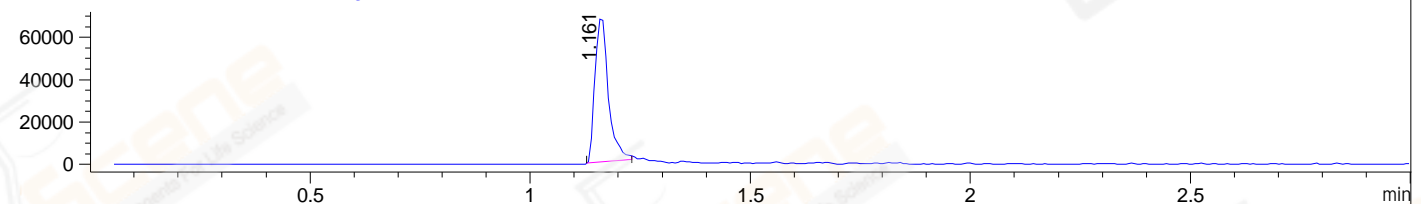

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.02	1221.29	910.17	99.92	378
1.21	0.01	0.93	1.99	0.08	376

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.02	779.44	595.90	99.91	378
1.23	0.01	0.68	0.77	0.09	376

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.04	536132.81	223764.03	100.00	378

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

