
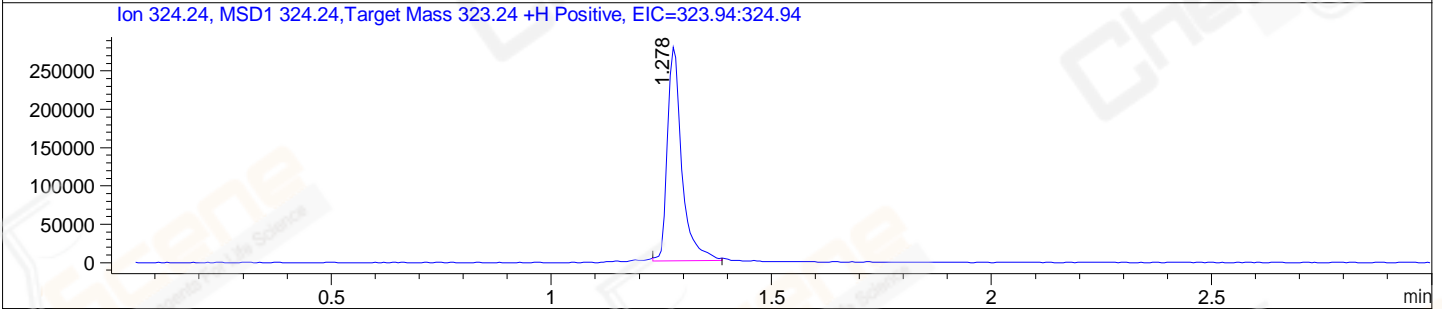
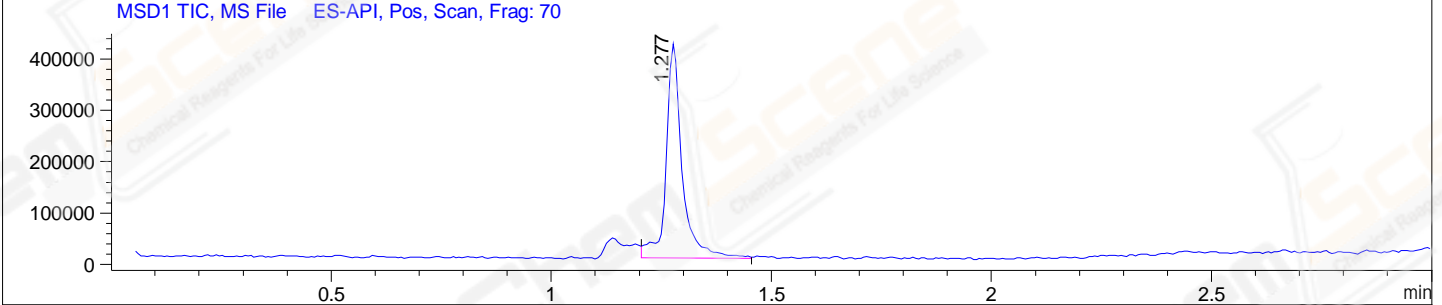


File ..1\DATA\2019\20190924\721\BIZ2019-923-SCH8.D Tgt Mass (CHM):
 Injection Date : 24 Sep 19 2:02 pm +0800 Seq. Line : 7
 Sample Name : BIZ2019-923-SCH8 Location : P1-D-05
 Acq. Operator : bgd_1571 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190924\721\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190924\721\1-POS-3MIN.M
 Catalog No : CS-4089 Batch#46213
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□

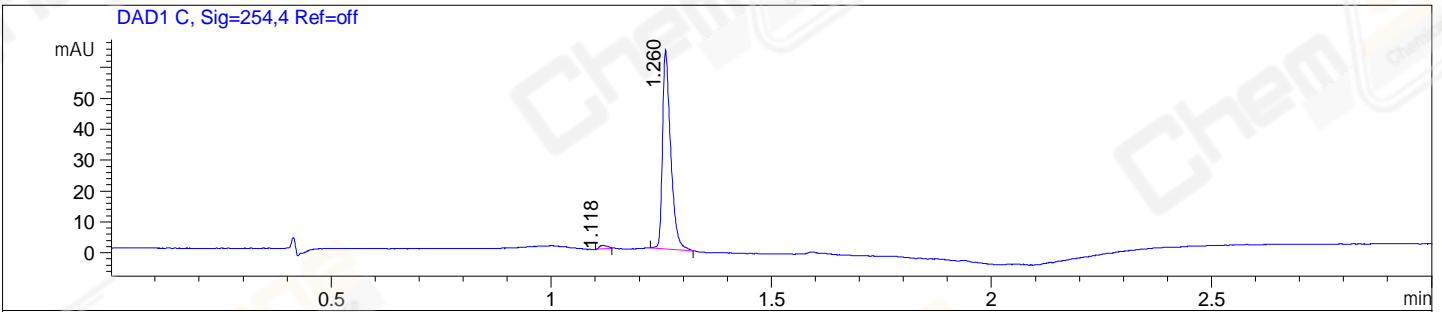

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.02	1.43	1.13	1.70	342
1.26	0.02	82.93	64.44	98.30	324

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.04	1068485.25	416917.72	100.00	324

Ret. Time: 1.28

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

