



File ..DATA\2019\20191225\796\BIZ2019-D24-SCH10-.D Tgt Mass (CHM):  
Injection Date : 25 Dec 19 11:59 pm +0800 Seq. Line : 68  
Sample Name : BIZ2019-D24-SCH10 Location : P1-D-07  
Acq. Operator : ZJ\_1432 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 0.5 ul  
Acq. Method : D:\Chem32\1\data\2019\20191225\796\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2019\20191225\796\1-POS-3MIN.M  
Catalog No : CS-0864 Batch#58177  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

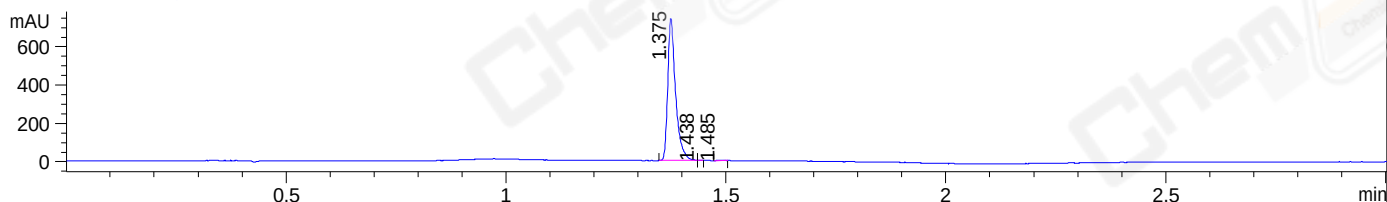


DAD1 C, Sig=254,4 Ref=off

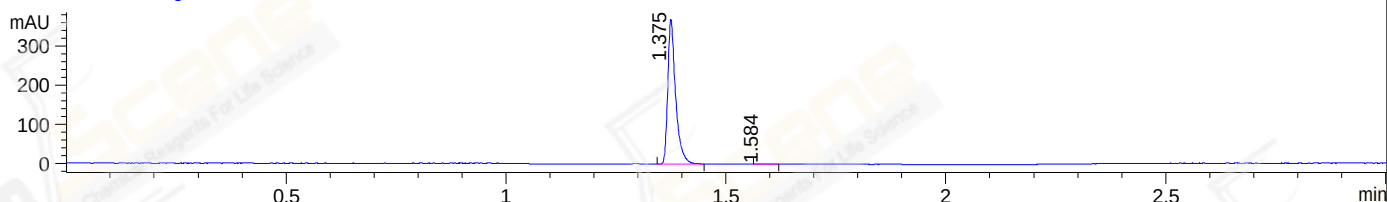

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

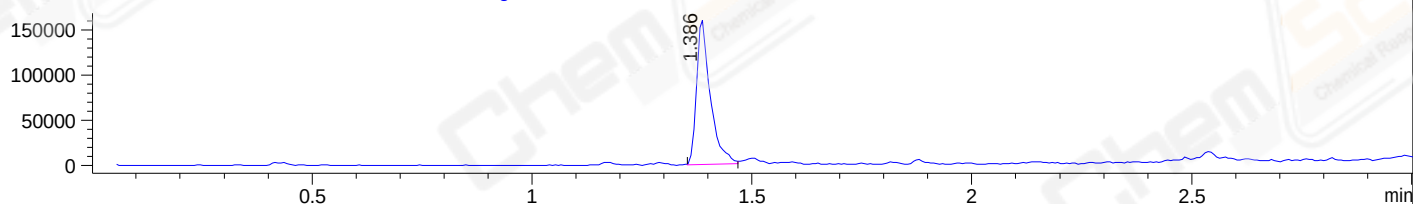

Ion 307, MSD1 307, Target Mass 306 +H Positive, EIC=306.7:307.7

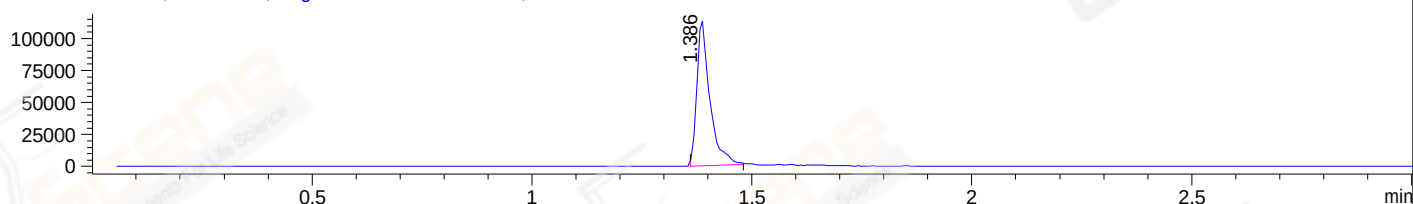

Integration Results for DAD1 B, Sig=214,4 Ref=off

| RetTim | Width | Area   | Height | Area% | MS (+) |
|--------|-------|--------|--------|-------|--------|
| 1.37   | 0.02  | 918.22 | 741.97 | 99.77 | 307    |
| 1.44   | 0.01  | 0.71   | 1.68   | 0.08  | 307    |
| 1.48   | 0.02  | 1.45   | 1.60   | 0.16  | 307    |

Integration Results for DAD1 C, Sig=254,4 Ref=off

| RetTim | Width | Area   | Height | Area% | MS (+) |
|--------|-------|--------|--------|-------|--------|
| 1.37   | 0.02  | 458.63 | 370.42 | 99.80 | 307    |
| 1.58   | 0.03  | 0.92   | 0.55   | 0.20  | 307    |

Integration Results for MSD1 TIC, MS File

| RetTim | Width | Area      | Height    | Area%  | MS (+) |
|--------|-------|-----------|-----------|--------|--------|
| 1.39   | 0.03  | 349864.75 | 161738.70 | 100.00 | 307    |

Ret. Time: 1.39

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

