



File ..1\DATA\2020\20200110\810\BIZ2020-109-SCH3.D Tgt Mass (CHM):
Injection Date : 10 Jan 20 8:04 pm +0800 Seq. Line : 63
Sample Name : BIZ2020-109-SCH3 Location : P1-A-06
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200110\810\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200110\810\1-POS-3MIN.M
Catalog No : CS-6150 Batch#58800
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

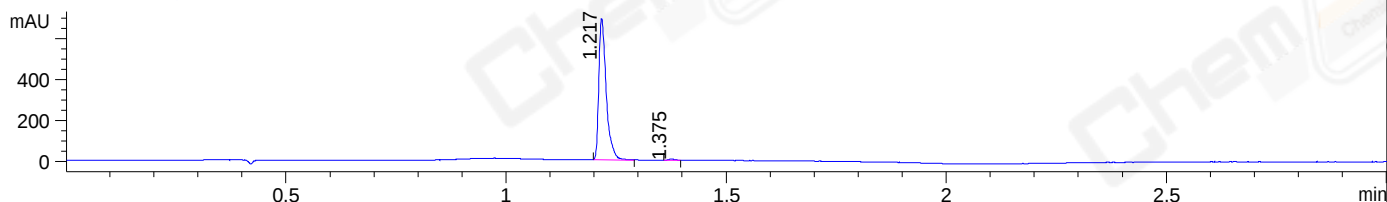


DAD1 C, Sig=254,4 Ref=off

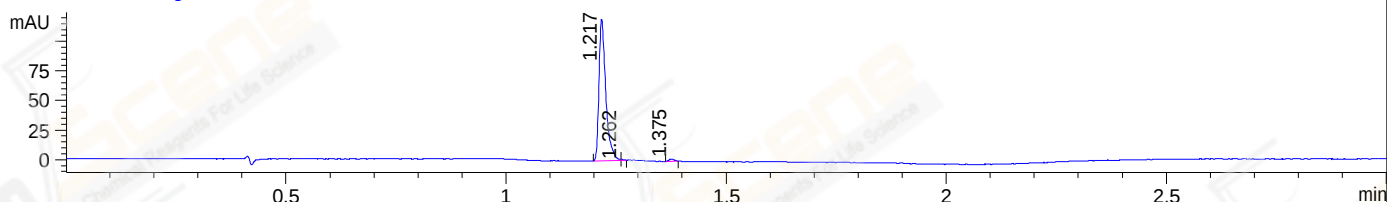

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

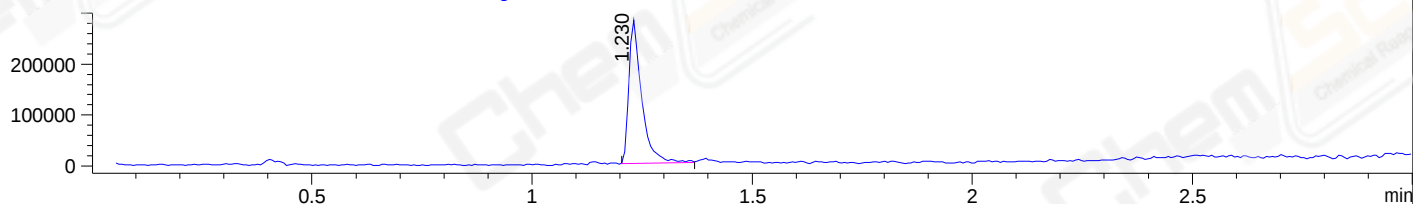

Ion 381, MSD1 381, Target Mass 380 +H Positive, EIC=380.7:381.7

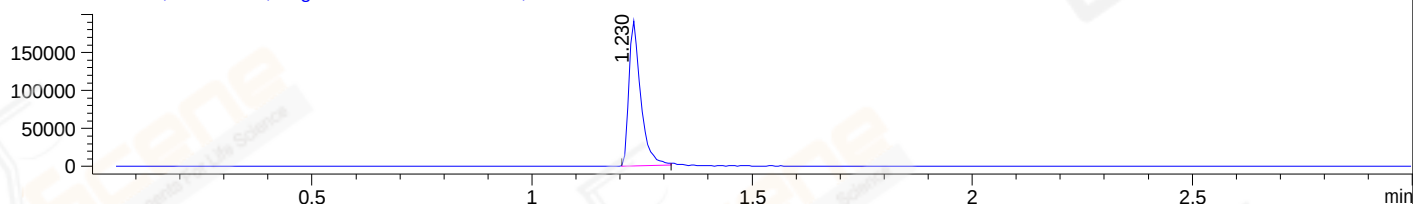

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	812.72	693.10	99.37	381
1.38	0.02	5.15	5.54	0.63	561

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	128.80	119.87	98.54	381
1.26	0.01	0.34	0.77	0.26	381
1.38	0.01	1.56	1.90	1.19	561

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.03	571479.75	280586.66	100.00	381

Ret. Time: 1.23

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

