



File ..ATA\2020\20200311\868 1\BIZ2020-312-SCH3-.D Tgt Mass (CHM):
 Injection Date : 13 Mar 20 4:51 pm +0800 Seq. Line : 4
 Sample Name : BIZ2020-312-SCH3 Location : P1-E-06
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\Chem32\1\data\2020\20200311\868 1\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200311\868 1\1-POS-3MIN.M
 Catalog No : CS-0039416
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

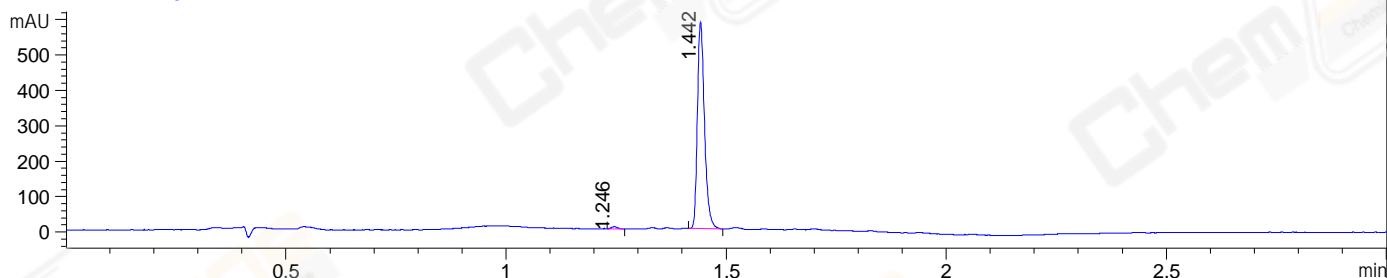

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

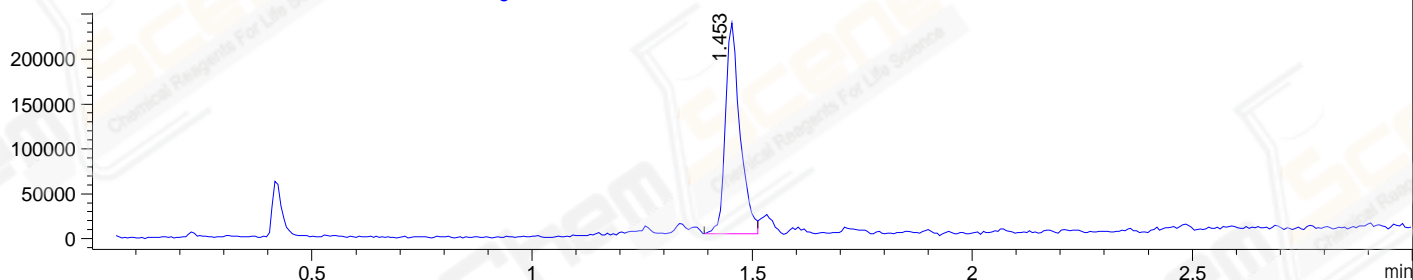

Ion 437, MSD1 437, Target Mass 436 +H Positive, EIC=436.7:437.7

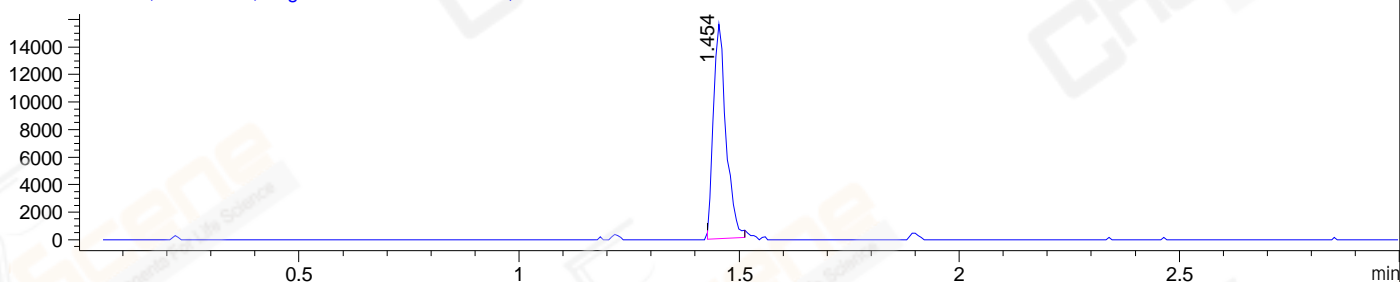

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	5.92	6.32	0.90	477
1.44	0.02	653.99	584.50	99.10	381

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.45	0.03	544546.00	235084.27	100.00	381

Ret. Time: 1.45

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

