

File ..\DATA\2023\20230317\875\BIZ2023-316-SCH1-.D Tgt Mass (CHM):

Injection Date : 17 Mar 23 5:40 pm +0800

Seq. Line : 116

Sample Name : BIZ2023-316-SCH1

Location : P1-A-05

Acq. Operator : ZJ_1432

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 0.5 uL

Acq. Method : D:\Chem32\1\data\2020\20200317\875\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200317\875\1-POS-3MIN.M

CAS NO. : 941678-49-5

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

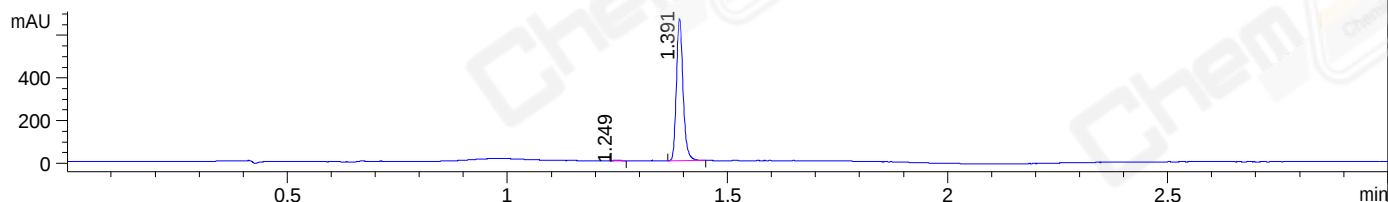


DAD1 C, Sig=254,4 Ref=off

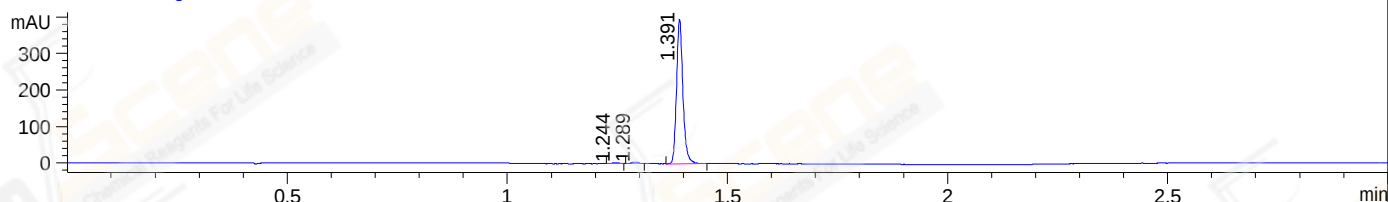

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

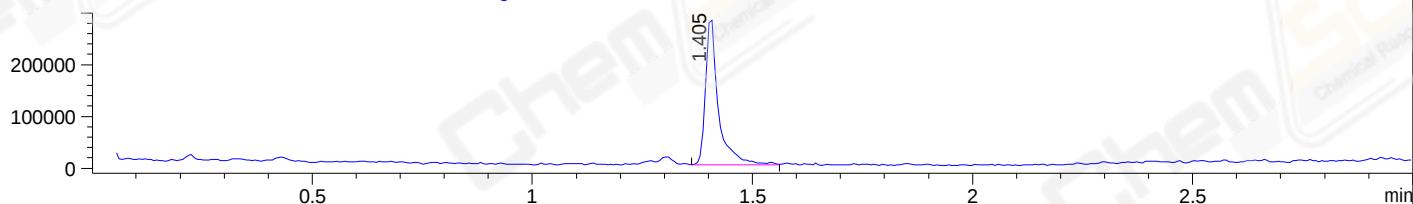

Ion 307, MSD1 307, Target Mass 306 +H Positive, EIC=306.7:307.7

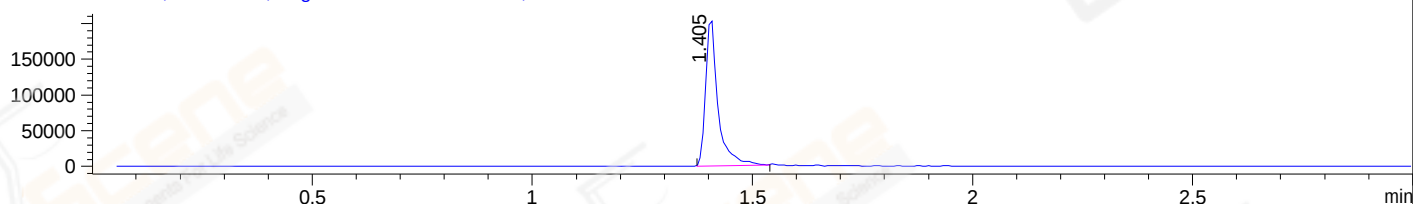

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.25	0.02	3.13	2.93	0.44	157
1.39	0.02	703.43	666.50	99.56	307

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.24	0.02	2.32	2.31	0.57	157
1.29	0.02	3.94	4.20	0.97	310
1.39	0.02	399.84	395.70	98.46	307

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.40	0.03	575442.88	287551.78	100.00	307

Ret. Time: 1.40

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

