



File ..DATA\2021\20210607\1411\CPK2021-604-61515.D Tgt Mass (CHM):
Injection Date : 7 Jun 21 11:38 am +0800 Seq. Line : 32
Sample Name : CPK2021-604-61515 Location : P1-B-06
Acq. Operator : wkt_2222 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 uL
Acq. Method : D:\Chem32\1\data\2021\20210607\1411\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210607\1411\1-POS-3MIN.M
CAS NO. : 941678-49-5
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

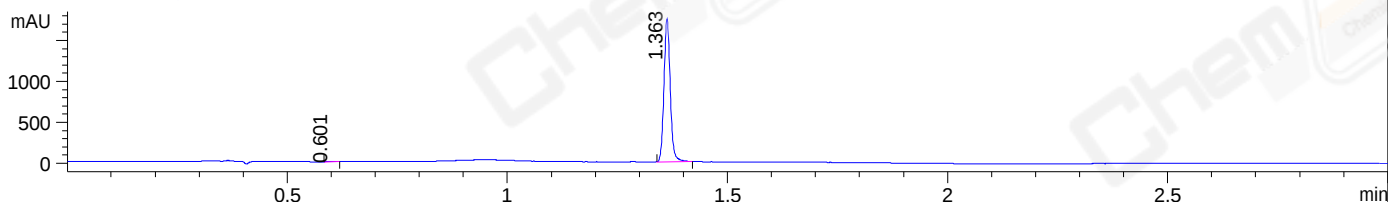


DAD1 C, Sig=254,4 Ref=off

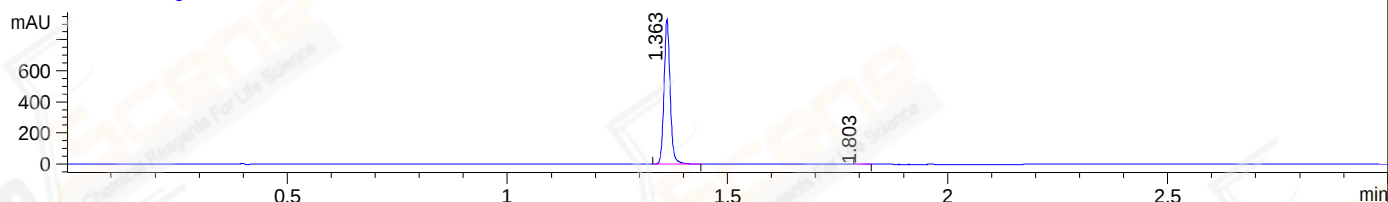

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

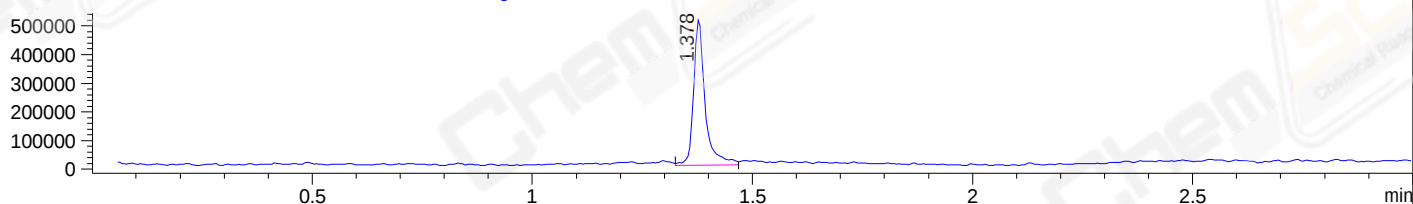

Ion 307, MSD1 307, Target Mass 306 +H Positive, EIC=306.7:307.7

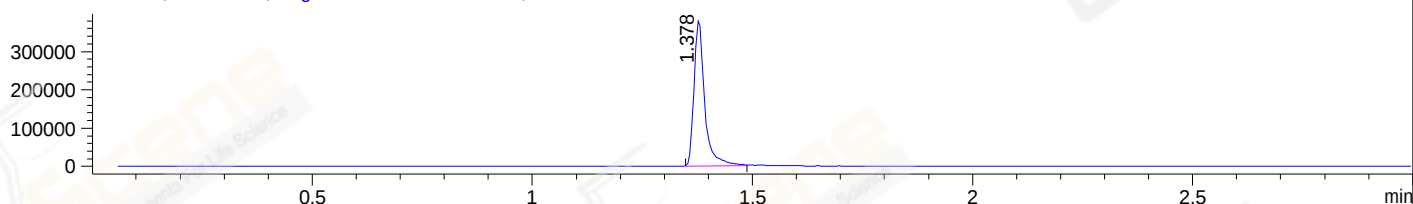

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
0.60	0.02	6.79	5.42	0.39	387
1.36	0.02	1733.47	1752.01	99.61	307

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.36	0.02	898.85	933.01	99.86	307
1.80	0.02	1.24	0.98	0.14	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.38	0.03	935198.56	510686.78	100.00	307

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

