



File ..\DATA\2020\20200326\896\BIZ2020-325-SCH7-.D Tgt Mass (CHM):  
Injection Date : 26 Mar 20 6:54 pm +0800 Seq. Line : 51  
Sample Name : BIZ2020-325-SCH7 Location : P1-C-04  
Acq. Operator : ZJ\_1432 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 0.5 ul  
Acq. Method : D:\Chem32\1\data\2020\20200326\896\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200326\896\1-POS-3MIN.M  
Catalog No : CS-6150 Batch#62149  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

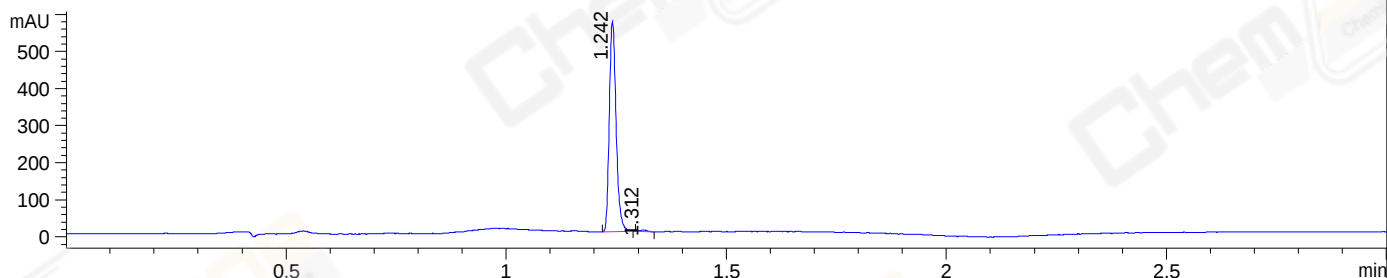

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

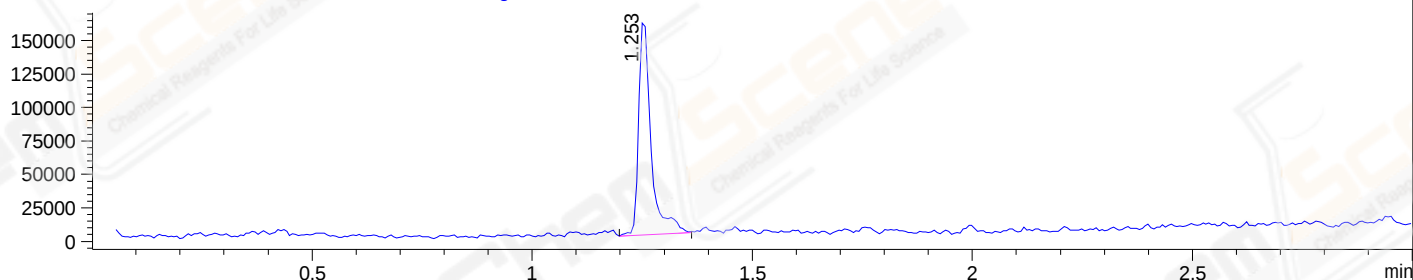

Ion 381, MSD1 381, Target Mass 380 +H Positive, EIC=380.7:381.7

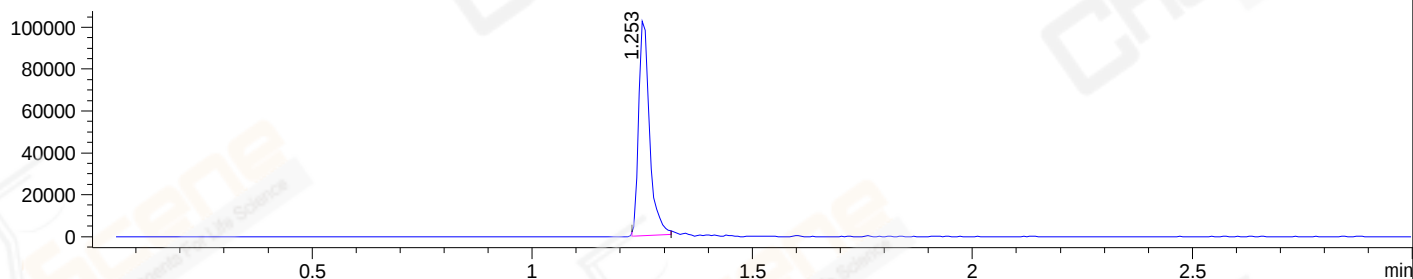

Integration Results for DAD1 B, Sig=214,4 Ref=off

| RetTim | Width | Area   | Height | Area% | MS (+) |
|--------|-------|--------|--------|-------|--------|
| 1.24   | 0.02  | 605.53 | 565.88 | 99.29 | 381    |
| 1.31   | 0.02  | 4.34   | 4.52   | 0.71  | 381    |

Integration Results for MSD1 TIC, MS File

| RetTim | Width | Area      | Height    | Area%  | MS (+) |
|--------|-------|-----------|-----------|--------|--------|
| 1.25   | 0.03  | 314190.69 | 163936.27 | 100.00 | 381    |

Ret. Time: 1.25

&lt;&lt;&lt;&lt; POSITIVE SPECTRA &gt;&gt;&gt;&gt;

ES-API Positive

