



File ..\DATA\2020\20200521\968\BIZ2020-520-CXL4.D Tgt Mass (CHM):
 Injection Date : 21 May 20 8:45 pm +0800 Seq. Line : 121
 Sample Name : BIZ2020-520-CXL4 Location : P1-D-04
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2020\20200521\968\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200521\968\1-POS-3MIN.M
 Catalog No : CS-0022885
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

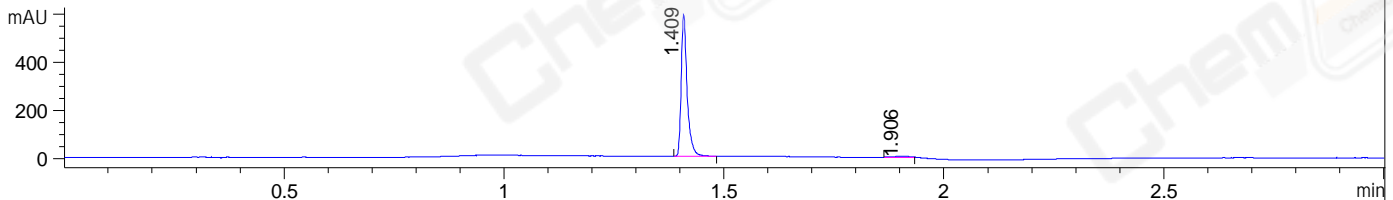


DAD1 C, Sig=254,4 Ref=off

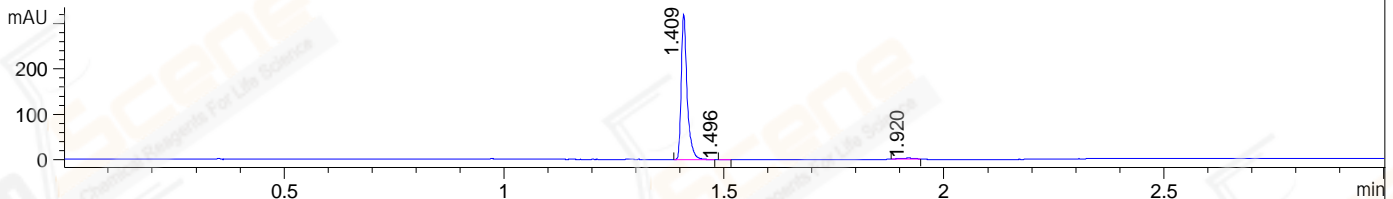

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

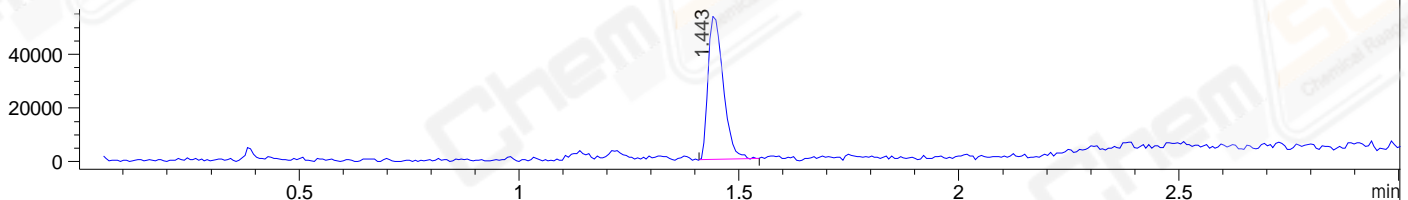

Ion 373, MSD1 373, Target Mass 372 +H Positive, EIC=372.7:373.7

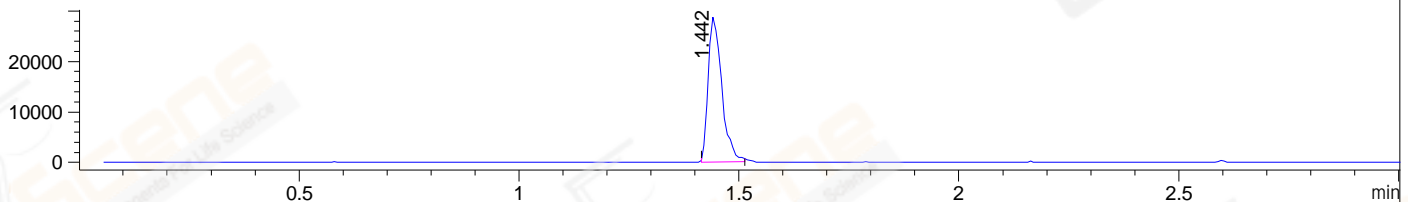

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.41	0.02	553.37	590.08	98.40	373
1.91	0.04	8.99	3.59	1.60	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.41	0.02	300.81	321.63	98.64	373
1.50	0.01	0.25	0.39	0.08	373
1.92	0.03	3.90	1.94	1.28	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.44	0.04	127664.52	54010.00	100.00	373

Ret. Time: 1.44

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

