



File ..\DATA\2020\20200521\968\BIZ2020-521-SCH2-.D Tgt Mass (CHM):  
 Injection Date : 21 May 20 9:17 pm +0800 Seq. Line : 128  
 Sample Name : BIZ2020-521-SCH2 Location : P1-E-02  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.5 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200521\968\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200521\968\1-POS-3MIN.M  
 Catalog No : CS-0008777  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

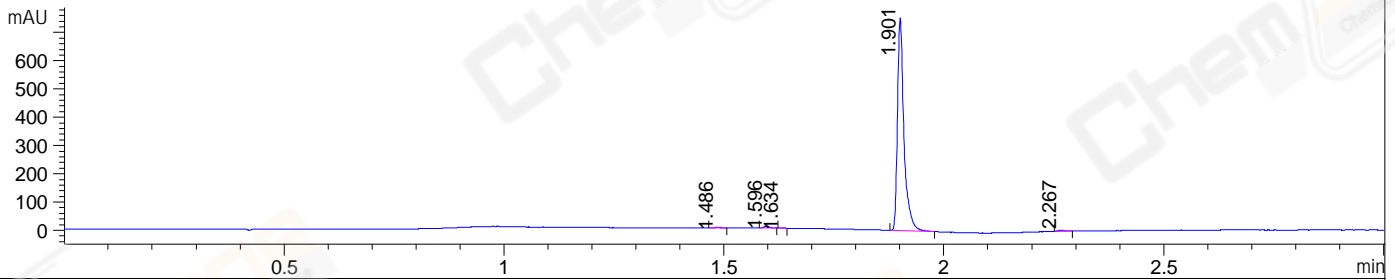

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

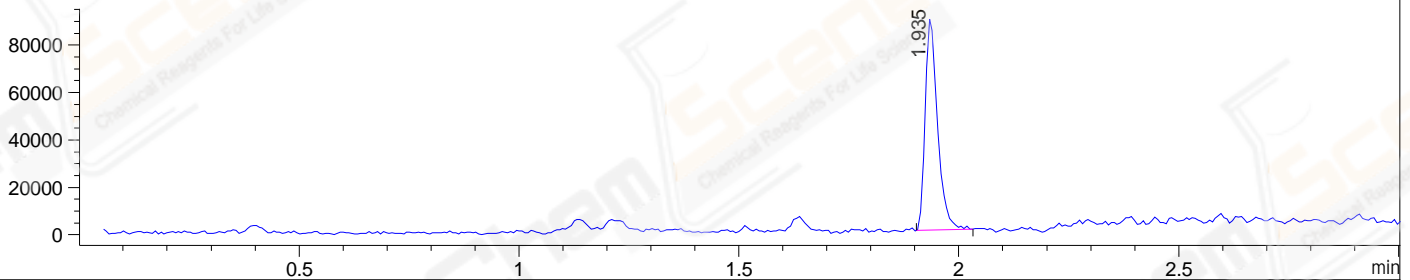

Ion 271, MSD1 271, Target Mass 270 +H Positive, EIC=270.7:271.7

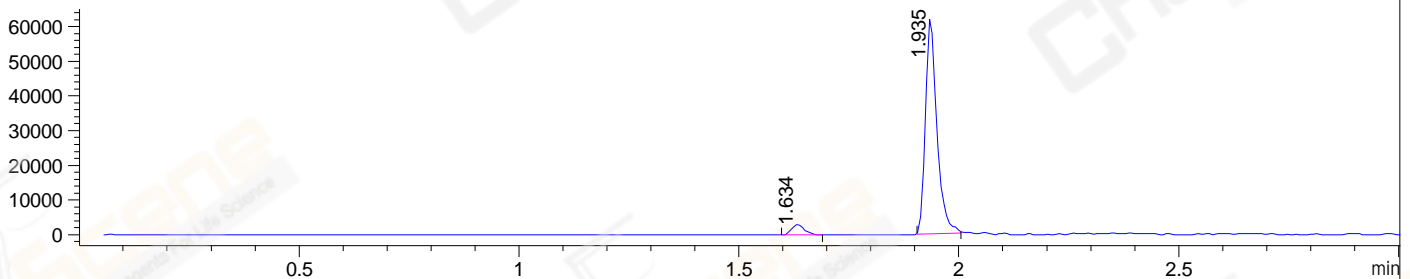

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.02	2.56	2.47	0.33	ND
1.60	0.01	5.83	6.76	0.74	ND
1.63	0.01	0.81	1.19	0.10	271
1.90	0.02	773.54	753.92	98.32	271
2.27	0.02	4.00	3.61	0.51	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.94	0.03	175521.70	90183.55	100.00	271

Ret. Time: 1.94

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

