



File E:\ChemStation\1\DATA\2025\2025-01\2025-01-21\CPK2025-0121-66621-UPLC-MS-10-053865.D
Injection Date : 21-Jan-25, 15:53:57 Tgt Mass(EZX) :
Sample Name : CPK2025-0121-66621 Location : P1-B-10
Acq. Operator : LY_2278 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.8 uL
Acq. Method : E:\ChemStation\1\Methods\1-POS-UPLC3.0MIN(1.2)(150-1000).M
Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-UPLC3.0MIN(1.2)(150-1000).M
CAS NO. : 950455-15-9 WalkUp method: '1-POS-3MIN' Project: CPK2025
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 2.0 min
Flow Rate :1.2ml/min
Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

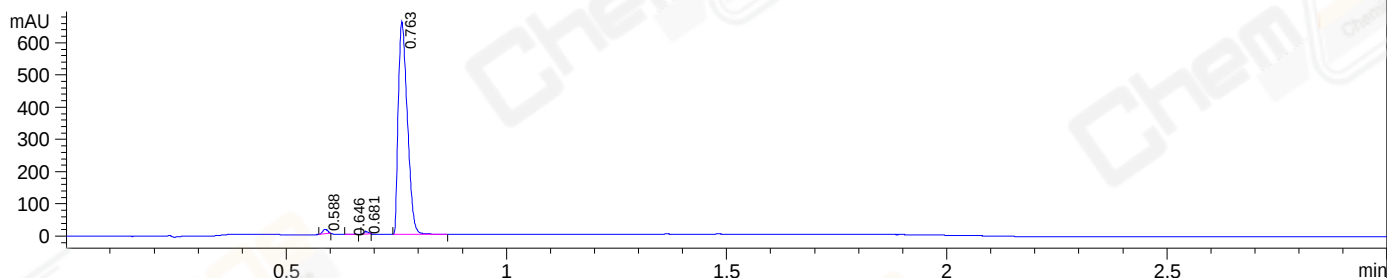

DAD1 B, Sig=254,4 Ref=off

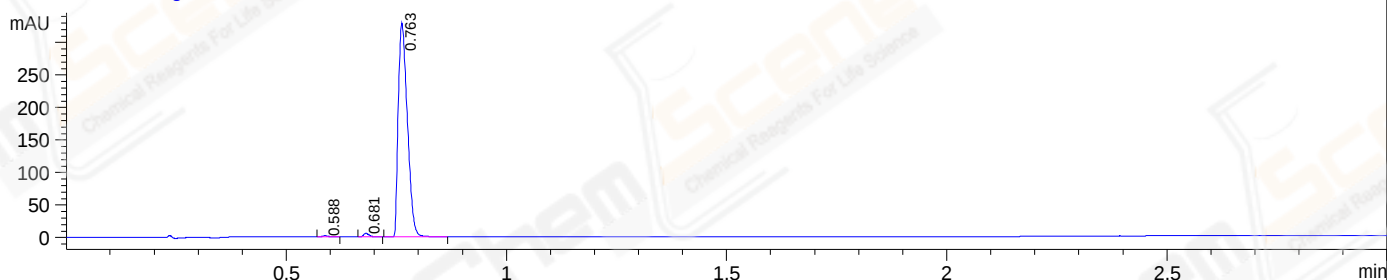

*MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

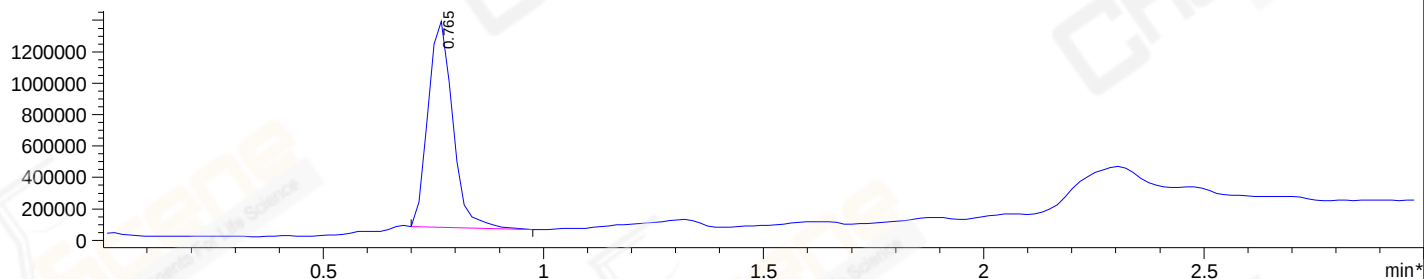

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.59	0.01	11.71	14.77	1.21
0.65	0.01	0.96	1.09	0.10
0.68	0.01	5.72	7.84	0.59
0.76	0.02	946.67	658.91	98.09

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
0.59	0.02	1.69	1.77	0.35
0.68	0.01	4.90	5.40	1.02
0.76	0.02	473.03	328.45	98.63

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
0.76	0.06	5110668.50	1322011.00	100.00

Ret. Time: 0.76

<<<< POSITIVE SPECTRA >>>>

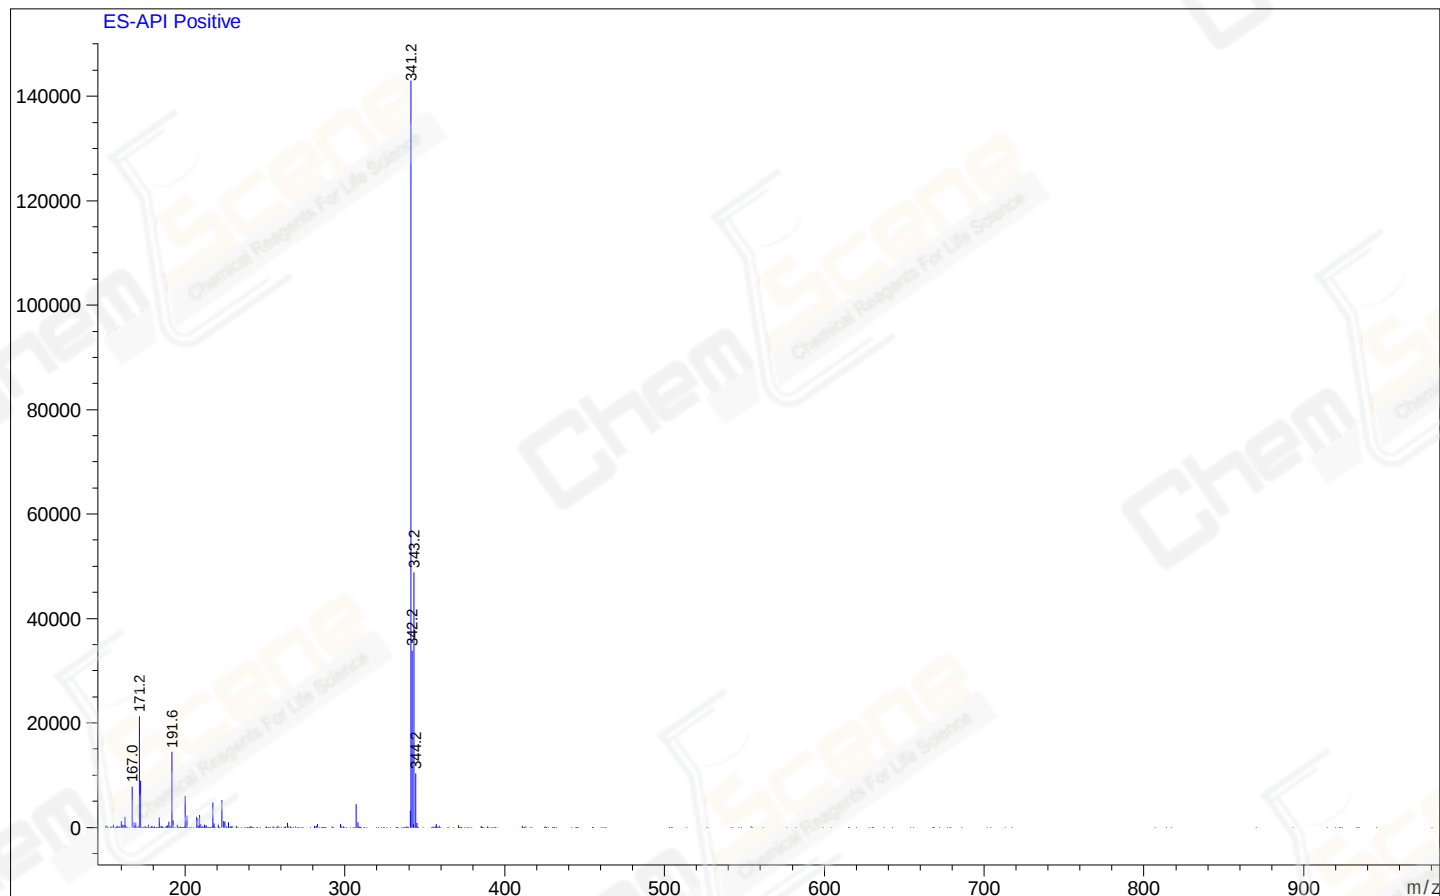

*** End of Report ***