



File ..\DATA\2020\20200707\1031\BIZ2020-706-SCH3.D Tgt Mass (CHM):
Injection Date : 7 Jul 20 10:12 am +0800 Seq. Line : 10
Sample Name : BIZ2020-706-SCH3 Location : P1-D-01
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.5 ul
Acq. Method : D:\Chem32\1\data\2020\20200707\1031\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200707\1031\1-POS-3MIN.M
Catalog No : CS-0864
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

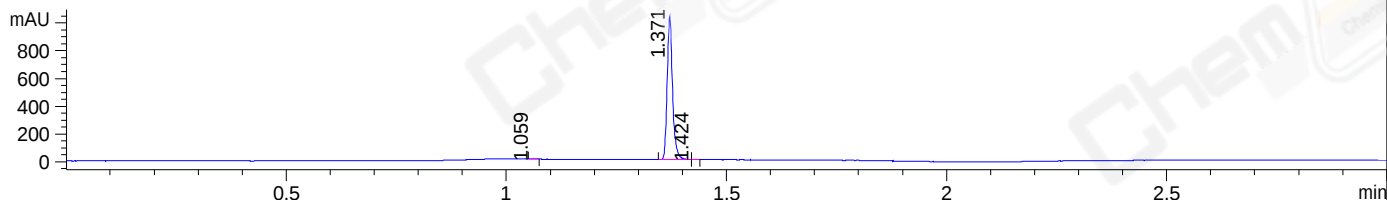


DAD1 C, Sig=254,4 Ref=off

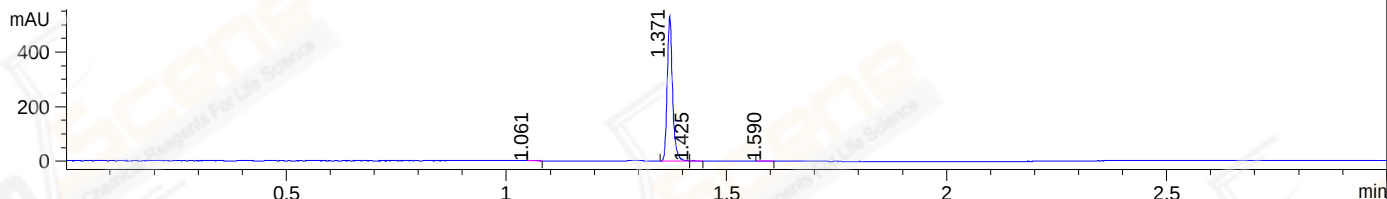

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

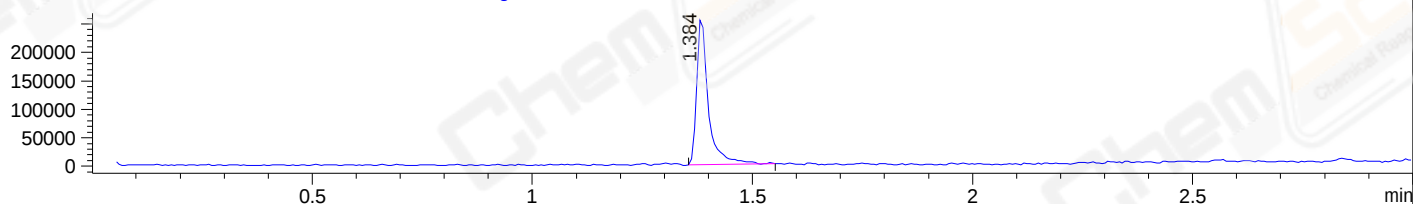

Ion 307, MSD1 307, Target Mass 306 +H Positive, EIC=306.7:307.7

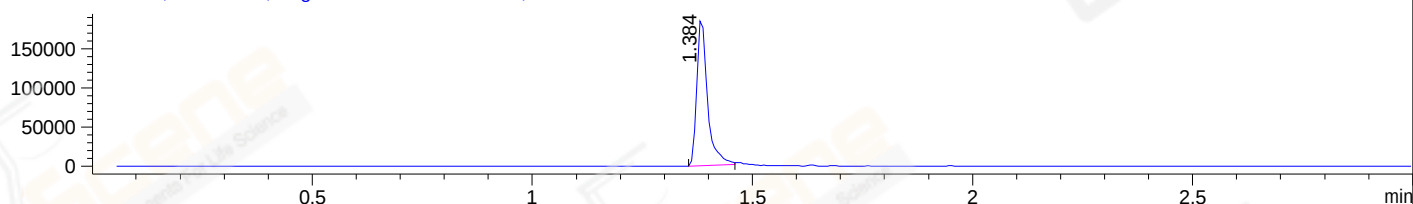

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.01	1.00	1.56	0.11	ND
1.37	0.01	874.29	1032.77	99.75	307
1.42	0.01	1.15	1.70	0.13	307

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.02	0.78	0.80	0.17	ND
1.37	0.01	445.06	531.72	99.32	307
1.42	0.02	1.27	1.29	0.28	307
1.59	0.02	0.99	0.80	0.22	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	475332.91	259758.98	100.00	307

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

