



File ..\DATA\2020\20200730\1058\BIZ2020-728-WLQ2.D Tgt Mass (CHM):
 Injection Date : 30 Jul 20 11:34 am +0800 Seq. Line : 33
 Sample Name : BIZ2020-728-WLQ2 Location : P1-A-02
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200730\1058\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200730\1058\1-POS-3MIN.M
 Catalog No : CS-4256
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

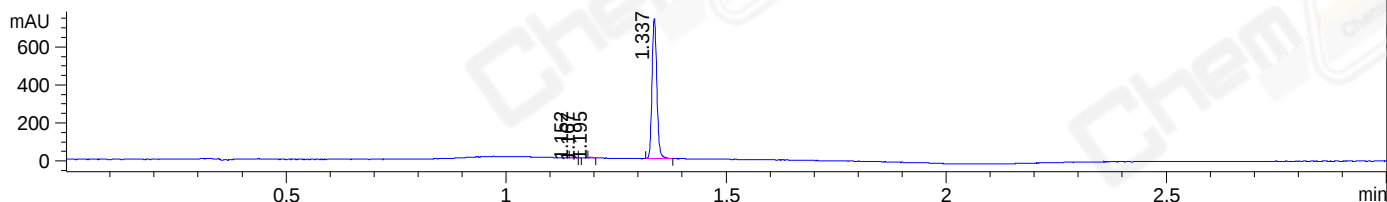


DAD1 C, Sig=254,4 Ref=off

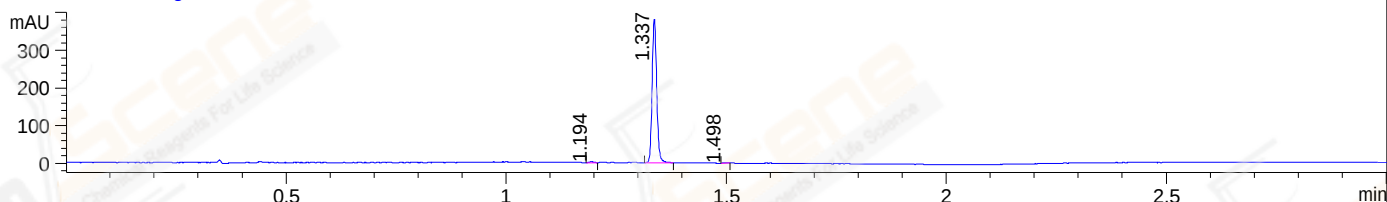

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

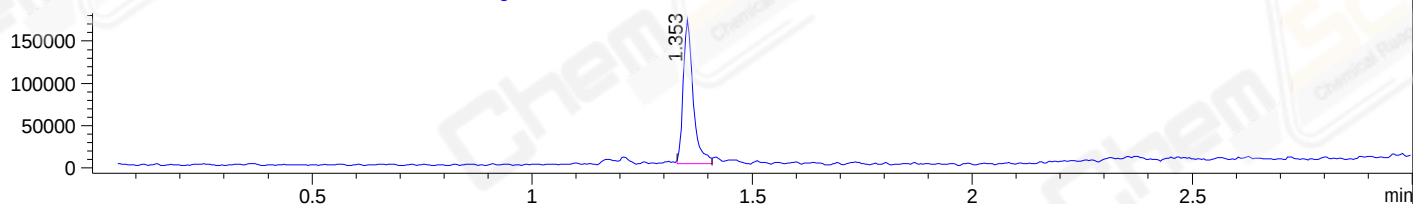

Ion 418, MSD1 418, Target Mass 417 +H Positive, EIC=417.7:418.7

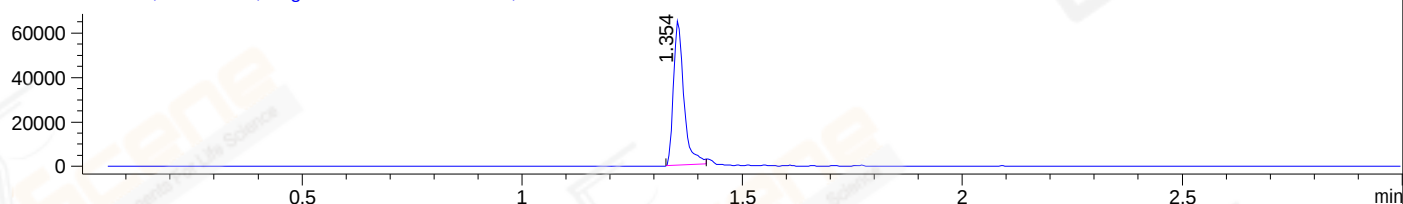

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.01	2.97	4.75	0.53	132
1.17	0.00	0.21	0.78	0.04	259
1.19	0.01	2.27	4.15	0.40	132
1.34	0.01	558.42	739.48	99.03	418

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.01	1.67	2.37	0.61	287
1.34	0.01	274.04	382.15	99.15	418
1.50	0.01	0.67	0.89	0.24	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.02	267106.09	169801.67	100.00	418

Ret. Time: 1.35

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

