



File ..\DATA\2020\20200819\1076\BIZ2020-817-WLQ3.D Tgt Mass (CHM):
 Injection Date : 19 Aug 20 8:34 pm +0800 Seq. Line : 121
 Sample Name : BIZ2020-817-WLQ3 Location : P1-A-03
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200819\1076\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200819\1076\1-POS-3MIN.M
 Catalog No : CS-1951
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

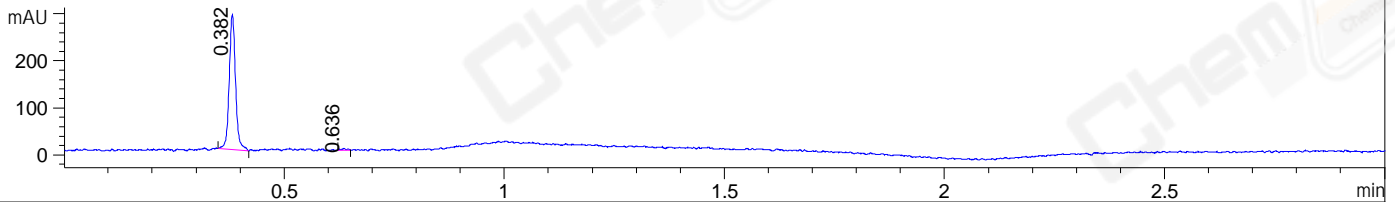


DAD1 C, Sig=254,4 Ref=off

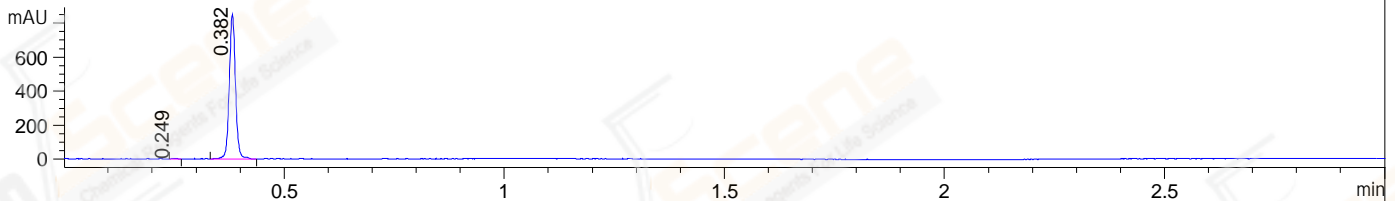

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

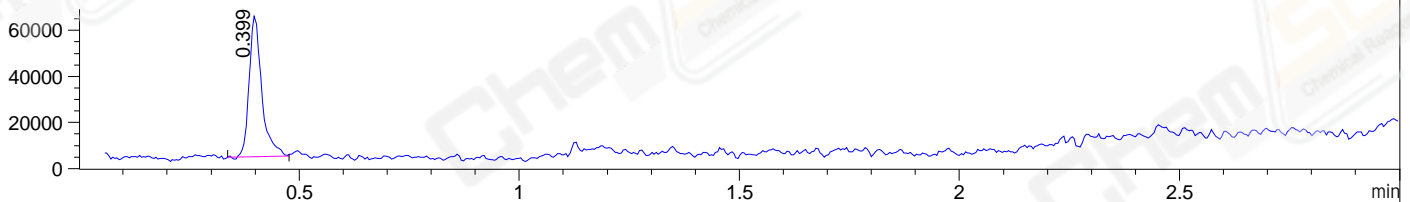

Ion 259, MSD1 259, Target Mass 258 +H Positive, EIC=258.7:259.7

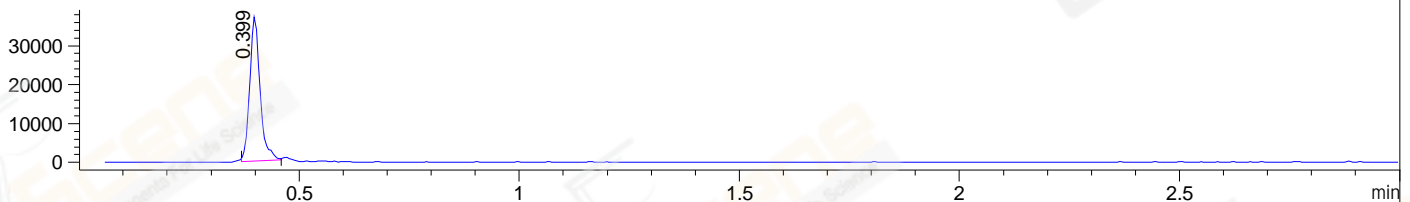

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.38	0.02	287.29	287.23	98.80	259
0.64	0.02	3.49	3.49	1.20	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.25	0.01	2.01	2.29	0.24	ND
0.38	0.02	836.01	850.80	99.76	259

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.40	0.03	122980.95	61161.10	100.00	259

Ret. Time: 0.40

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

