



File ..\DATA\2020\20200822\1080\BIZ2020-821-WMX1.D Tgt Mass (CHM):  
Injection Date : 22 Aug 20 9:27 am +0800 Seq. Line : 6  
Sample Name : BIZ2020-821-WMX1 Location : P1-A-04  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200822\1080\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200822\1080\1-POS-3MIN.M  
Catalog No : CS-0026698  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

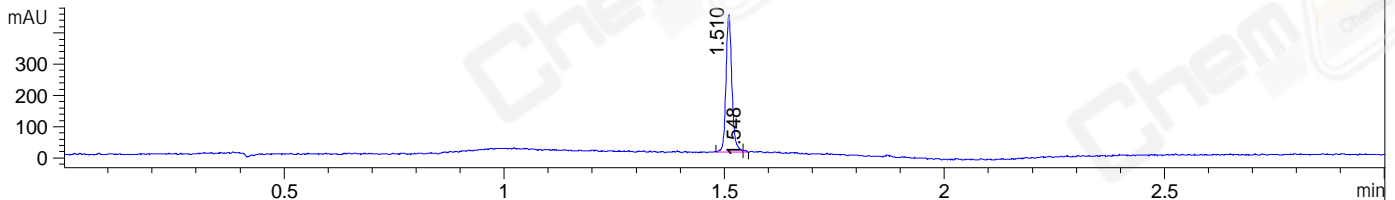


DAD1 C, Sig=254,4 Ref=off

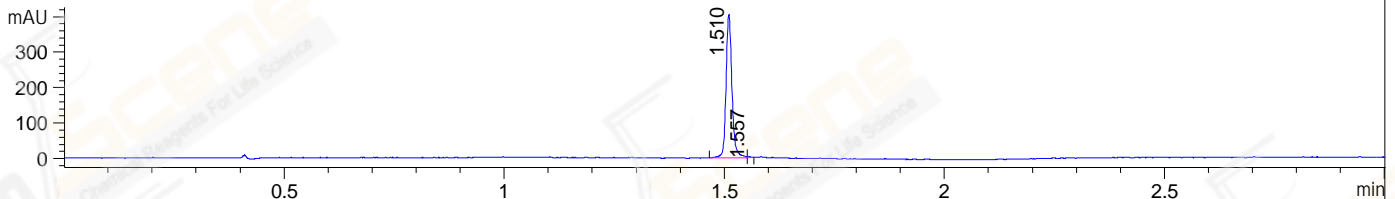

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

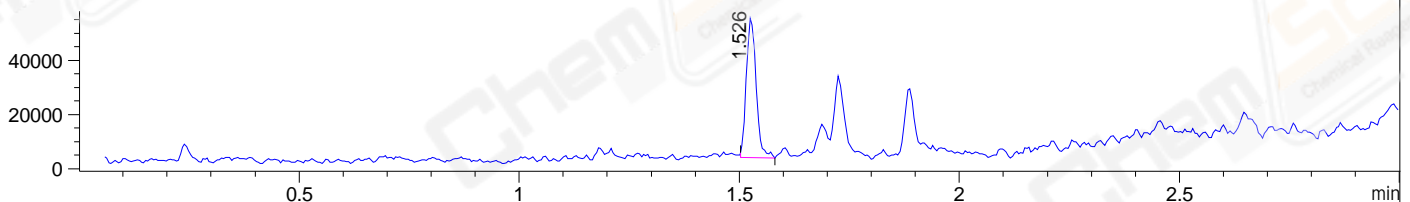

Ion 266, MSD1 266, Target Mass 265 +H Positive, EIC=265.7:266.7

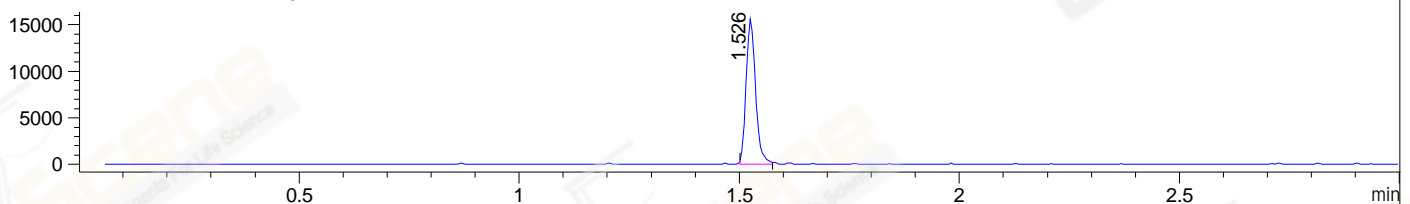

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.02	407.03	441.25	99.32	266
1.55	0.01	2.80	5.76	0.68	266

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.02	374.95	405.20	99.68	266
1.56	0.01	1.21	2.37	0.32	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.53	0.03	80378.73	51893.46	100.00	266

Ret. Time: 1.53

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

