



File ..\DATA\2020\20200819\1076\BIZ2020-818-SCH7.D Tgt Mass (CHM):  
 Injection Date : 19 Aug 20 9:40 pm +0800 Seq. Line : 135  
 Sample Name : BIZ2020-818-SCH7 Location : P1-B-08  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200819\1076\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200819\1076\1-POS-3MIN.M  
 Catalog No : CS-1110  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

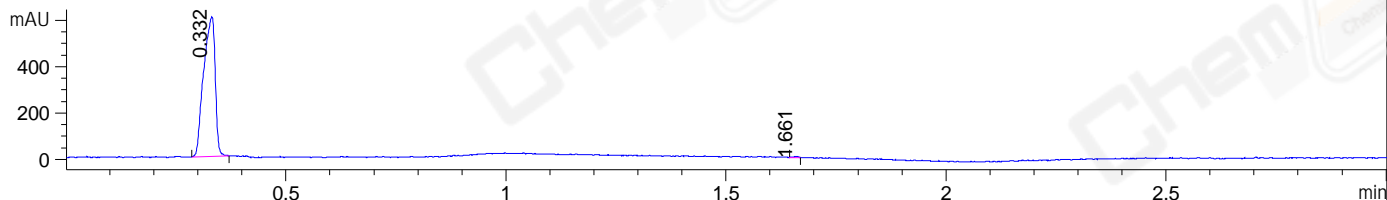


DAD1 C, Sig=254,4 Ref=off

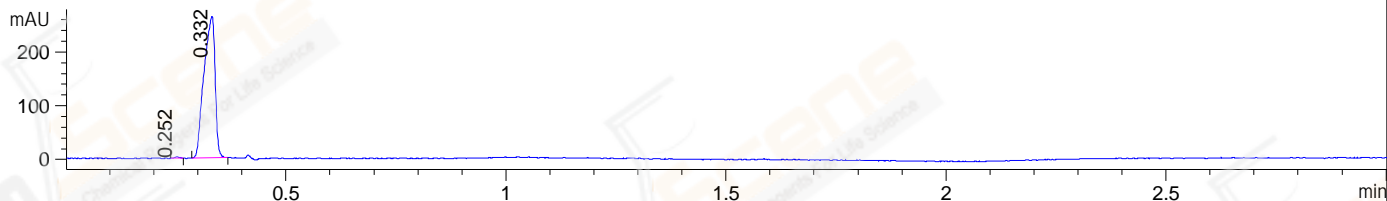

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

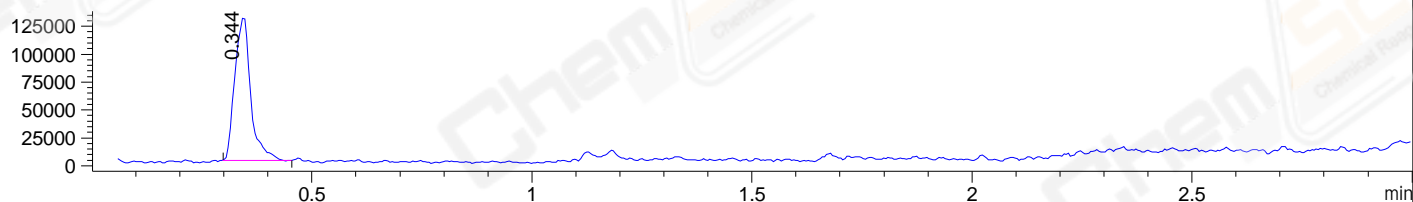

Ion 212, MSD1 212, Target Mass 211 +H Positive, EIC=211.7:212.7

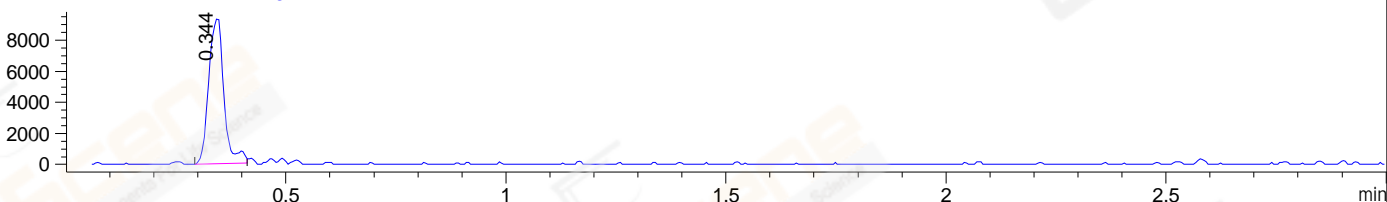

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
0.33	0.03	1095.26	603.17	99.61	423
1.66	0.02	4.30	4.73	0.39	217

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
0.25	0.01	1.92	2.53	0.41	ND
0.33	0.03	461.65	263.47	99.59	423

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
0.34	0.04	322630.84	128526.38	100.00	423

Ret. Time: 0.34

<<<< POSITIVE SPECTRA >>>>

