

File E:\ChemStation\1\DATA\2023-06\2023-06-06\CPK2023-605-81887-LCMS-20-005384.D

Injection Date : 06-Jun-23, 13:21:32

Tgt Mass(EZX) :

Sample Name : CPK2023-605-81887

Location : P1-D-01

Acq. Operator : LY_2278

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 1 uL

Acq. Method : E:\ChemStation\1\Methods\1-POS-2MIN(1.5ML)-(150-1000).M

Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-2MIN(1.5ML)-(150-1000).M

CAS NO. : 49627-27-2 WalkUp method: '1-POS-2MIN(150-1000)' Project: CPK2023


Method Info : Mobile Phase: A: water(0.01%FA) B:ACN(0.01%FA)

Flow Rate :1.5ml/min


Column :Shim-pack Scepter C18-120, 3.0*33mm,3um

Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

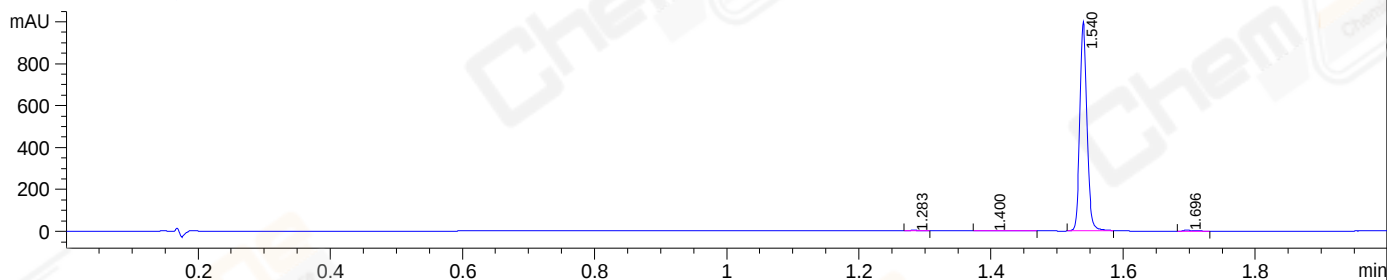

DAD1 B, Sig=254,4 Ref=off

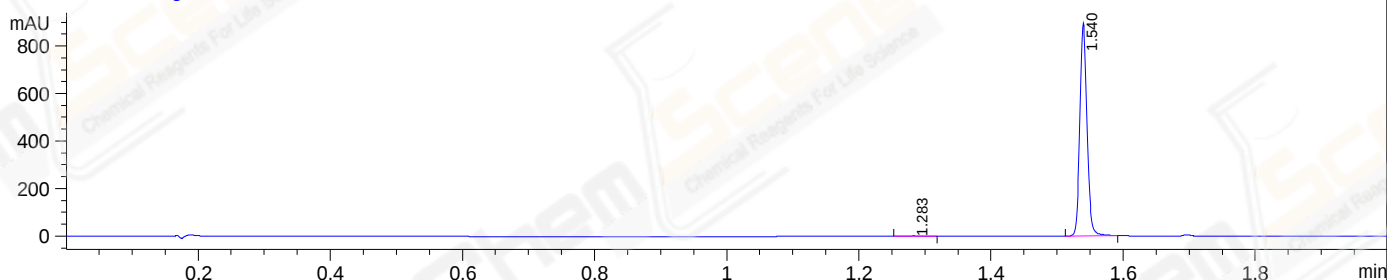

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

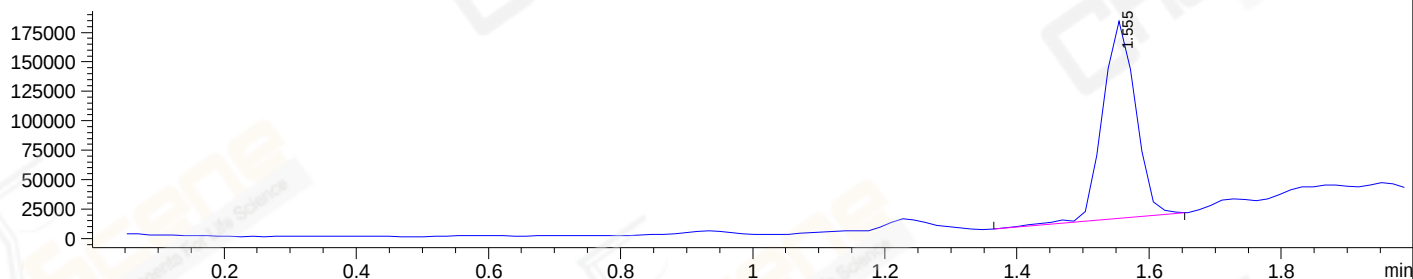

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.28	0.01	1.62	2.28	0.21
1.40	0.03	1.72	0.85	0.22
1.54	0.01	755.32	997.69	98.60
1.70	0.02	7.37	6.51	0.96

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
1.28	0.01	1.31	1.71	0.19
1.54	0.01	680.10	896.54	99.81

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
1.55	0.06	583572.56	167148.91	100.00

Ret. Time: 1.55

<<<< POSITIVE SPECTRA >>>>

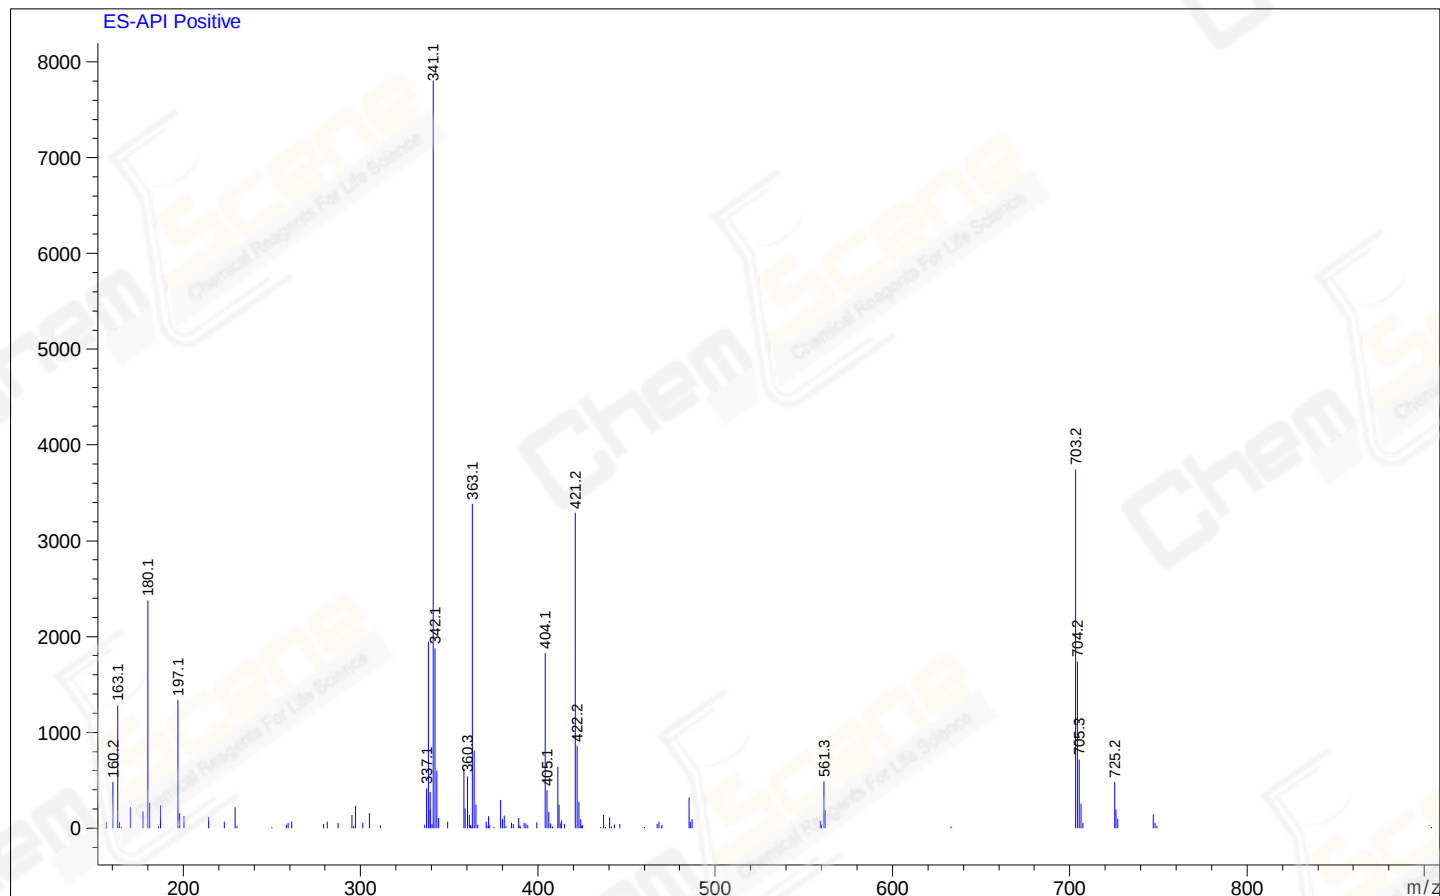

*** End of Report ***