



File ..\DATA\2020\20201019\1129\BIZ2020-O15-SCH1.D Tgt Mass (CHM):
 Injection Date : 19 Oct 20 12:20 pm +0800 Seq. Line : 41
 Sample Name : BIZ2020-O15-SCH1 Location : P1-A-01
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201019\1129\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201019\1129\1-POS-3MIN.M
 Catalog No : CS-7513
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

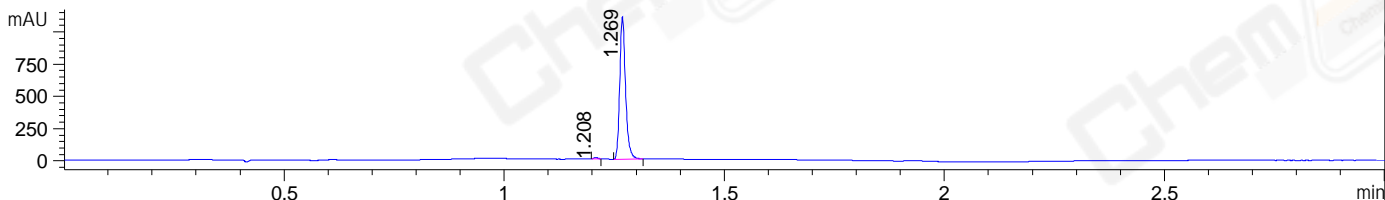


DAD1 C, Sig=254,4 Ref=off

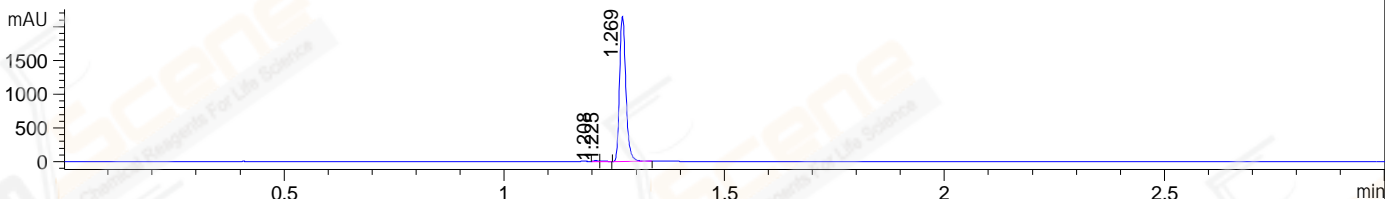

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

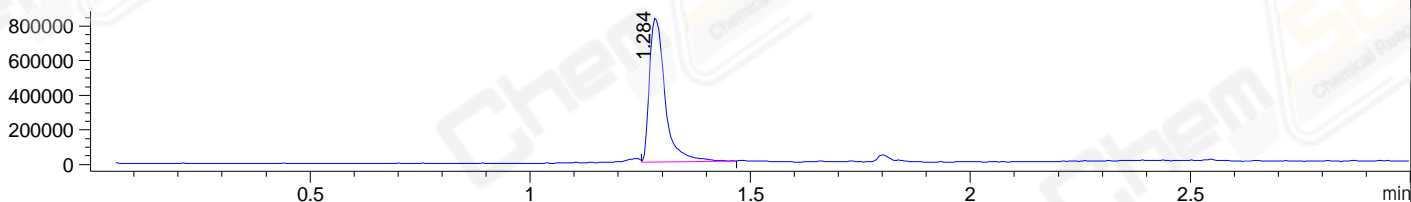

Ion 302, MSD1 302, Target Mass 301 +H Positive, EIC=301.7:302.7

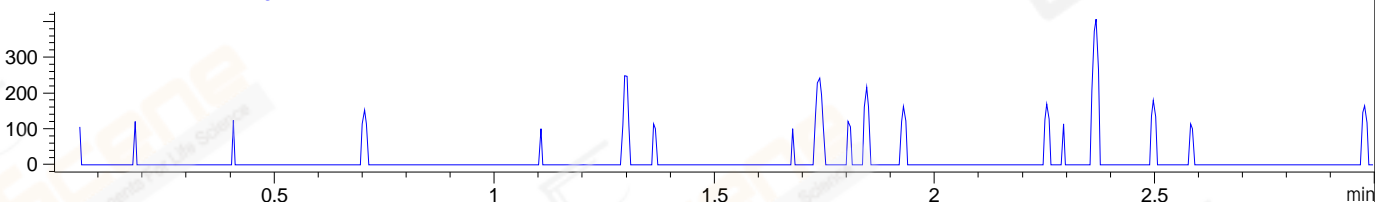

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.21	0.01	6.73	11.21	0.66	367
1.27	0.02	1014.89	1107.57	99.34	266

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.21	0.01	7.33	11.07	0.34	367
1.23	0.01	7.31	9.24	0.34	252
1.27	0.02	2159.94	2151.80	99.33	266

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.28	0.04	2060611.38	836280.38	100.00	266

Ret. Time: 1.28

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

