



File ..\DATA\2020\20201022\1133\BIZ2020-O20-WLQ3.D Tgt Mass (CHM):
Injection Date : 22 Oct 20 8:08 pm +0800 Seq. Line : 65
Sample Name : BIZ2020-O20-WLQ3 Location : P1-B-04
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201022\1133\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201022\1133\1-POS-3MIN.M
CAS NO. : 1351761-44-8
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

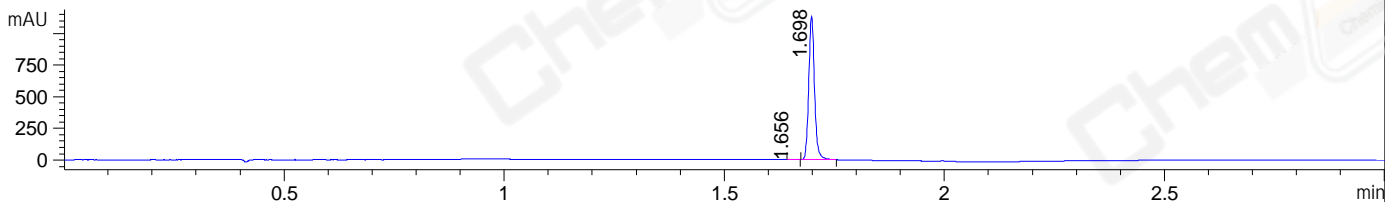


DAD1 C, Sig=254,4 Ref=off

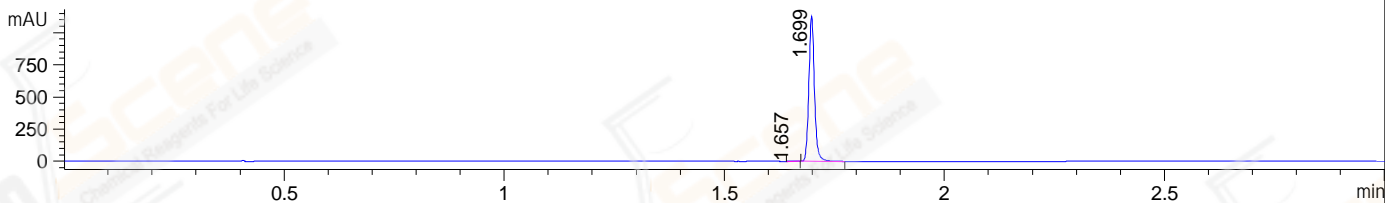

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

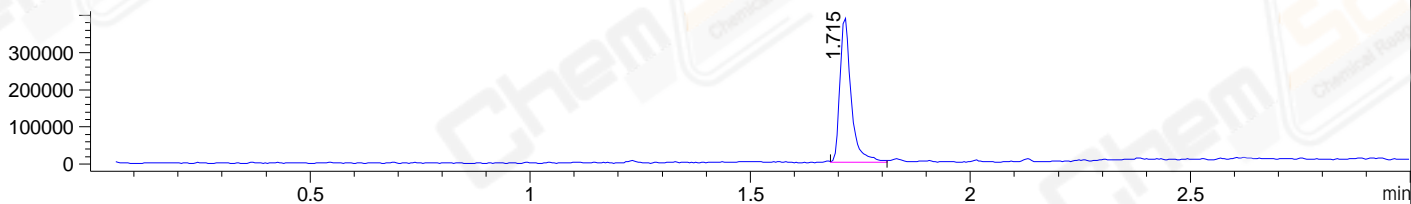

Ion 444, MSD1 444, Target Mass 443 +H Positive, EIC=443.7:444.7

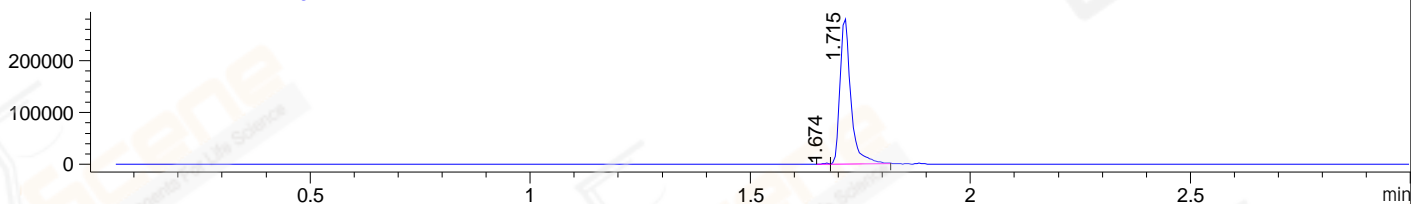

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.66	0.02	2.21	1.91	0.21	ND
1.70	0.02	1033.76	1132.57	99.79	444

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.66	0.02	1.49	1.28	0.15	ND
1.70	0.01	1005.52	1130.48	99.85	444

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.71	0.03	694319.62	390488.78	100.00	444

Ret. Time: 1.71

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

