



File ..\DATA\2020\20201102\1142\BIZ2020-O30-WMX5.D Tgt Mass (CHM):
Injection Date : 2 Nov 20 1:35 pm +0800 Seq. Line : 51
Sample Name : BIZ2020-O30-WMX5 Location : P1-A-03
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201102\1142\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201102\1142\1-POS-3MIN.M
Catalog No : CS-0101412
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

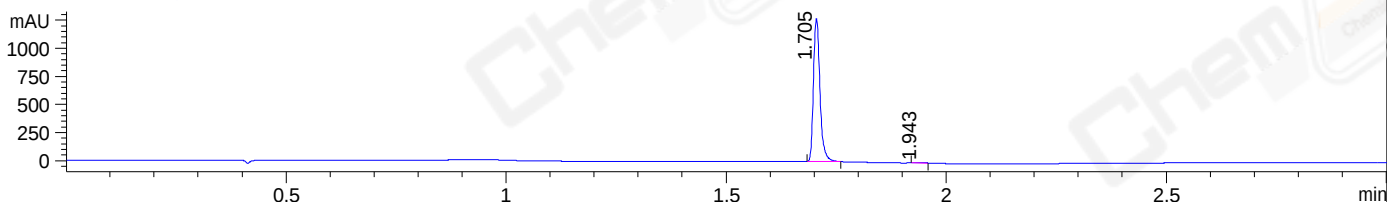


DAD1 C, Sig=254,4 Ref=off

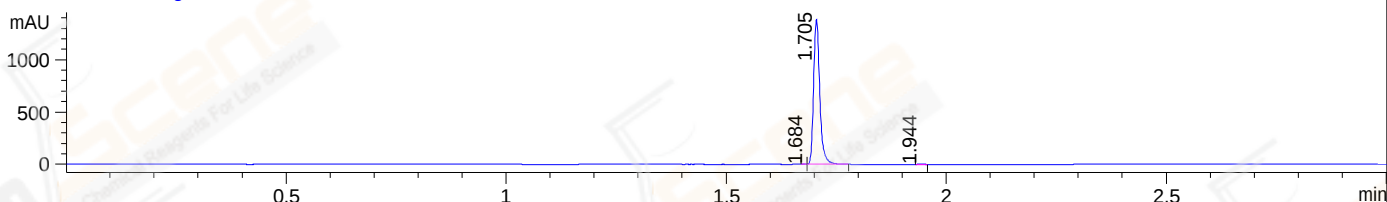

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

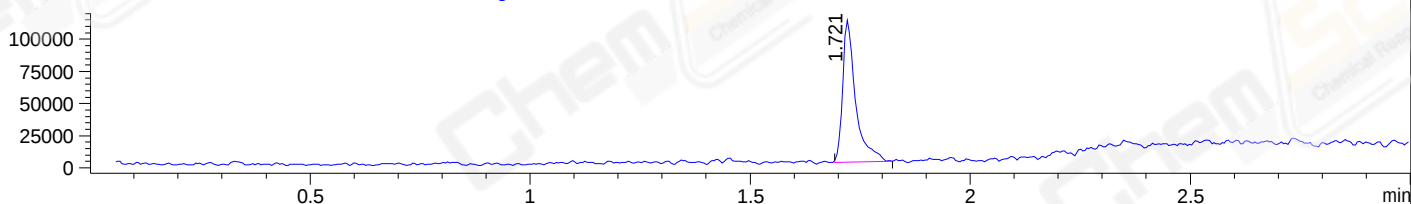

Ion 585, MSD1 585, Target Mass 584 +H Positive, EIC=584.7:585.7

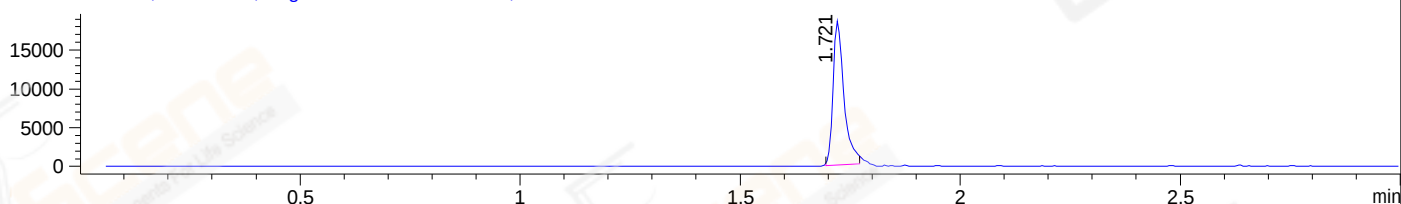

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.71	0.02	1303.59	1273.51	99.61	584
1.94	0.02	5.08	4.50	0.39	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.68	0.01	1.12	2.28	0.08	ND
1.71	0.02	1351.16	1390.62	99.70	584
1.94	0.01	2.93	3.28	0.22	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.72	0.03	225002.44	110342.20	100.00	584

Ret. Time: 1.72

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

