



File ..\DATA\2020\20201113\1152\BIZ2020-N12-SCH1.D Tgt Mass (CHM):  
 Injection Date : 13 Nov 20 3:11 pm +0800 Seq. Line : 70  
 Sample Name : BIZ2020-N12-SCH1 Location : P1-A-01  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20201113\1152\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20201113\1152\1-POS-3MIN.M  
 Catalog No : CS-0087276  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

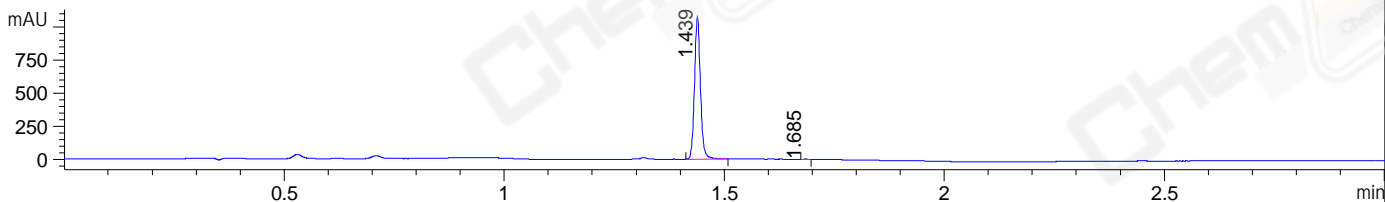


DAD1 C, Sig=254,4 Ref=off

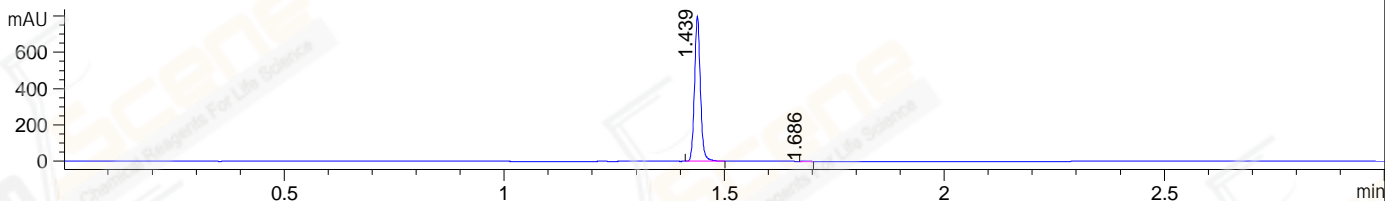

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

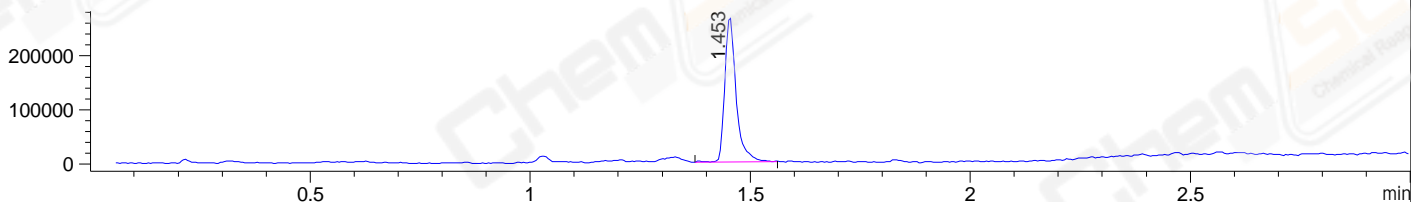

Ion 265, MSD1 265, Target Mass 264 +H Positive, EIC=264.7:265.7

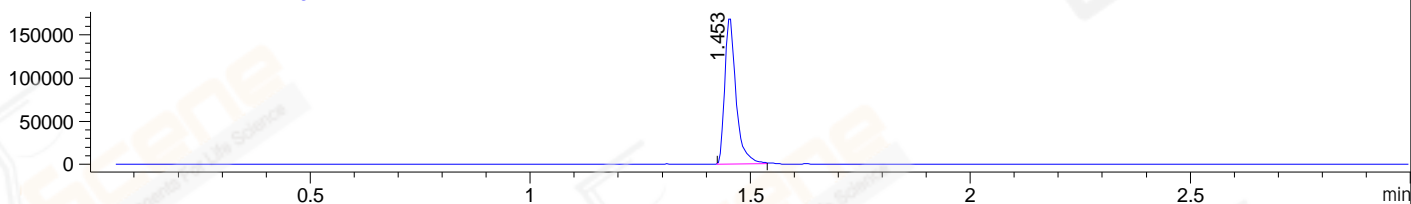

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.44	0.02	1014.81	1081.67	99.85	265
1.69	0.01	1.54	1.91	0.15	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.44	0.02	744.81	801.92	99.86	265
1.69	0.01	1.07	1.25	0.14	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.45	0.03	481895.78	269113.13	100.00	265

Ret. Time: 1.45

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

