



File ..\DATA\2020\20201113\1152\BIZ2020-N12-SCH3.D Tgt Mass (CHM):
Injection Date : 13 Nov 20 4:12 pm +0800 Seq. Line : 83
Sample Name : BIZ2020-N12-SCH3 Location : P1-D-02
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201113\1152\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201113\1152\1-POS-3MIN.M
CAS NO. : 170569-86-5
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

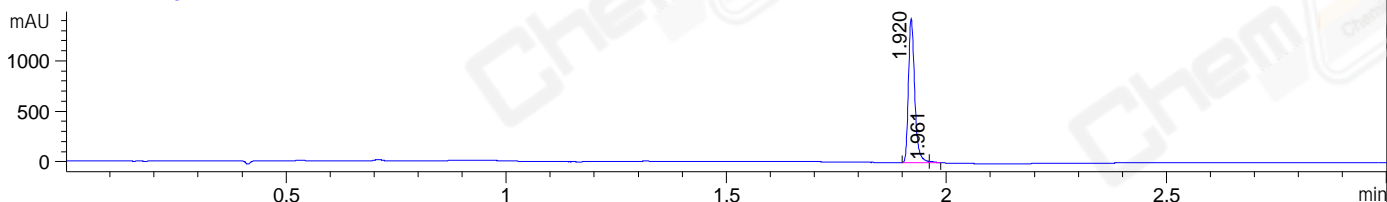


DAD1 C, Sig=254,4 Ref=off

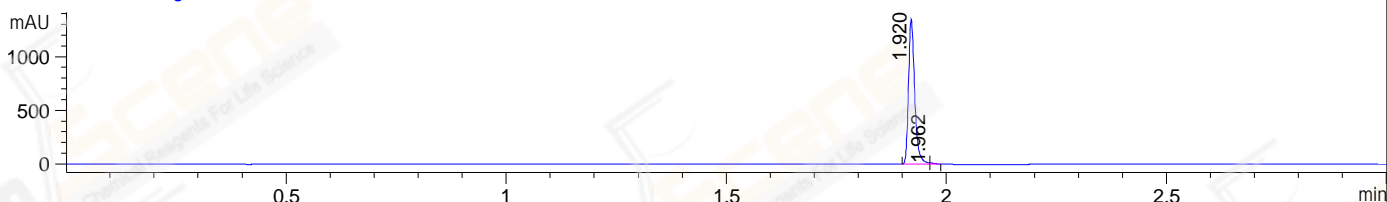

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

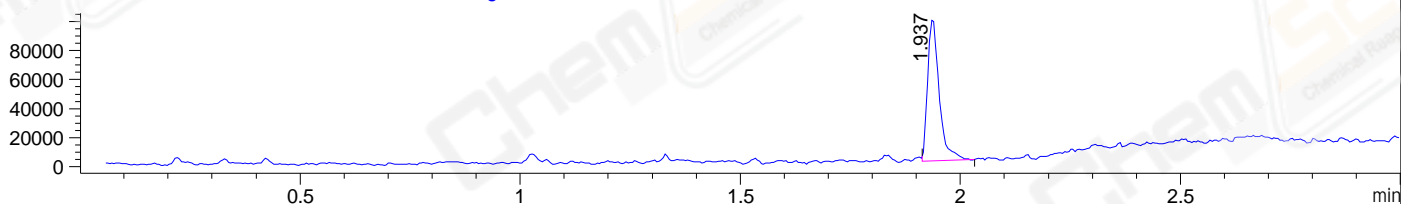

Ion 402, MSD1 402, Target Mass 401 +H Positive, EIC=401.7:402.7

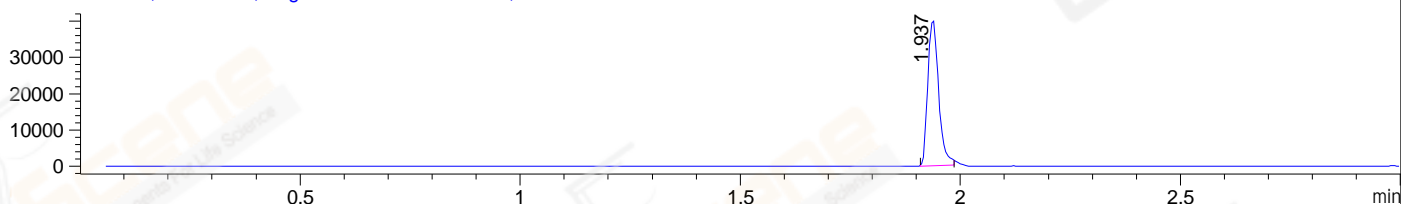

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.92	0.02	1417.98	1432.98	99.24	402
1.96	0.01	10.79	14.02	0.76	402

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.92	0.02	1316.46	1351.92	99.36	402
1.96	0.01	8.43	11.98	0.64	402

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.94	0.03	178408.22	98443.63	100.00	402

Ret. Time: 1.94

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

