



File ..\DATA\2021\20210114\1235\BIZ2021-114-SCH2.D Tgt Mass (CHM):

Injection Date : 14 Jan 21 3:09 pm +0800 Seq. Line : 55
 Sample Name : BIZ2021-114-SCH2 Location : P1-A-01
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 uL
 Acq. Method : D:\Chem32\1\data\2021\20210114\1235\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210114\1235\1-POS-3MIN.M
 CAS NO. : 1417997-93-3
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

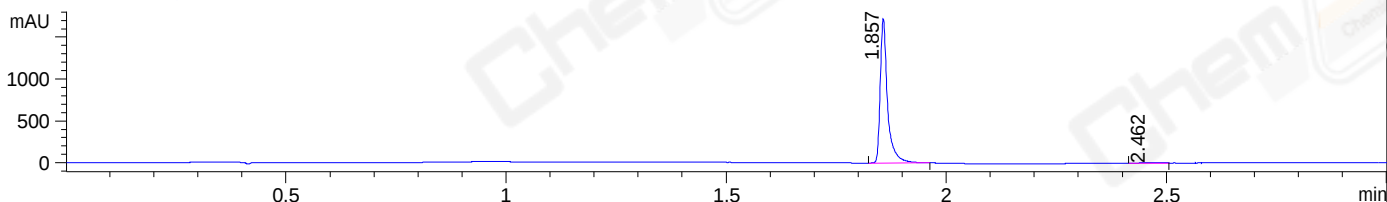


DAD1 C, Sig=254,4 Ref=off

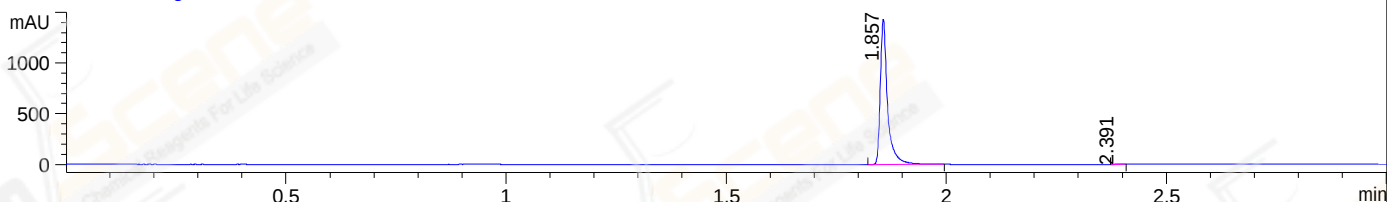

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

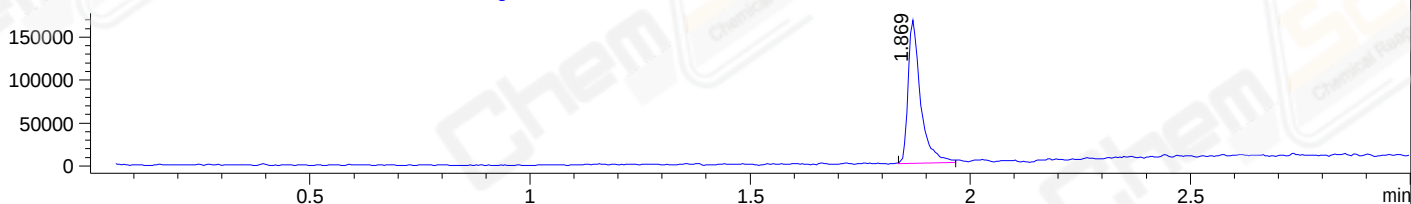

Ion 346, MSD1 346, Target Mass 345 +H Positive, EIC=345.7:346.7

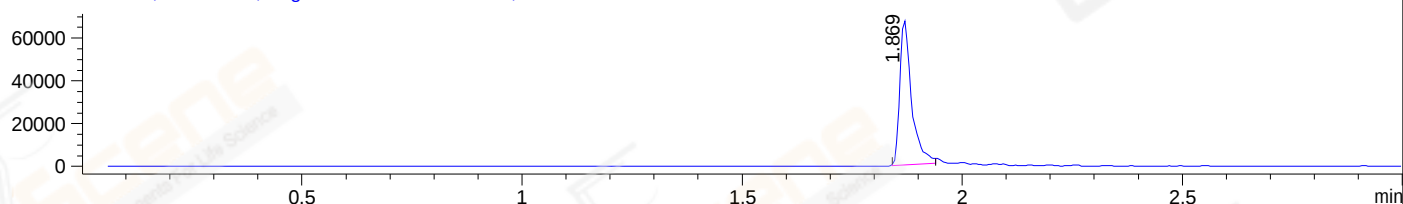

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.86	0.02	1984.79	1727.16	99.75	346
2.46	0.06	5.06	1.36	0.25	305

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.86	0.02	1647.00	1434.13	99.95	346
2.39	0.02	0.76	0.63	0.05	305

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.87	0.03	329586.69	166490.72	100.00	346

Ret. Time: 1.87

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

