




Chromatogram and Results

Anhui haoyuan Pharmaceutical Co.,Ltd

Injection Name: LJC202011090113
Vial Number: RB1
Injection Type: Unknown
Calibration Level: AHM003
Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0
Processing Method: LJC202011090113
seq.creation_operator Mbaogd
CAS NO.: 882847-34-9 575.65

Channel: TIC_POS
Wavelength: 220.0
Injection Volume: 1.00
Injection Time: 10/11/2020 09:59
InstMeth.creation_time 28/08/2020 09:10
Last update_time: 10/Nov/2020 13:01
Data Operator: Mbaogd
Print Operator: Mbaogd

chrom://ahqc009/XVault/AHM003/42/20201110-1.seq/223.smp/TIC_POS.channel/TIC_POS.chm

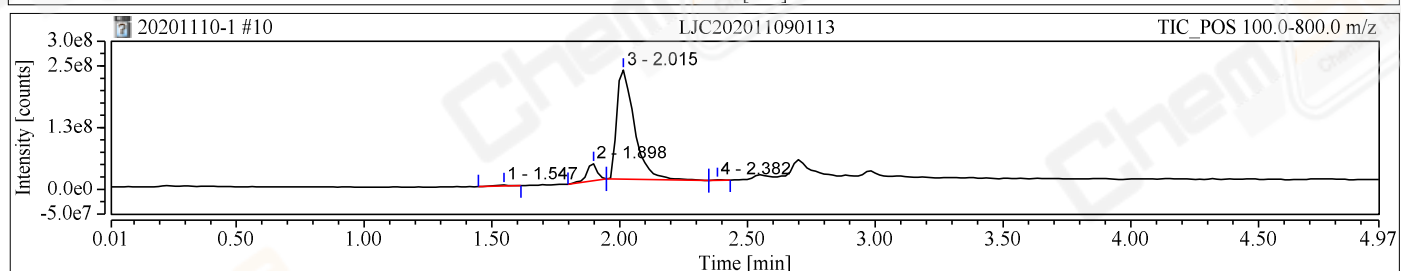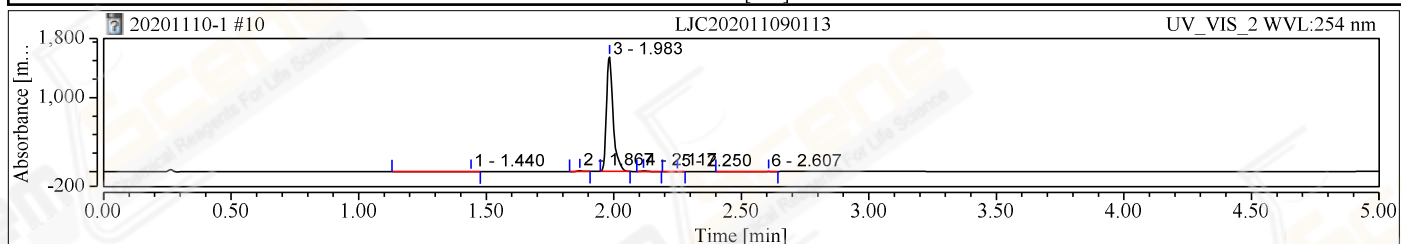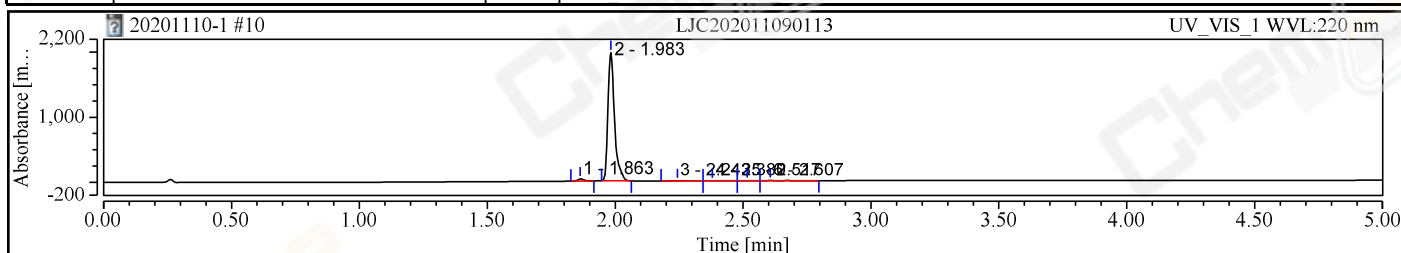


Peak Results for UV_VIS_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	1.863	0.918	34.179	31612	2.78	1.48	1.54	
2	1.983	58.401	1968.786	32053	2.26	1.47	98.03	
3	2.243	0.057	0.554	2322	1.16	1.34	0.10	
4	2.380	0.058	1.216	38019	2.35	1.93	0.10	
5	2.517	0.021	0.494	22199	1.60	1.14	0.03	
6	2.607	0.122	1.962	53742	n.a.	3.22	0.21	
Total:		59.577	2007.191	179947.000	10.15			

Peak Results for UV_VIS_2

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	1.440	0.052	0.138	144	1.64	0.54	0.11	
2	1.867	0.255	10.301	34686	2.75	1.05	0.55	
3	1.983	46.141	1544.279	31429	3.06	1.46	98.71	
4	2.117	0.254	8.967	39800	2.58	1.76	0.54	
5	2.250	0.017	0.351	21815	4.72	0.73	0.04	
6	2.607	0.025	0.107	13365	n.a.	0.57	0.05	
Total:		46.744	1564.144	141239.000	14.75			

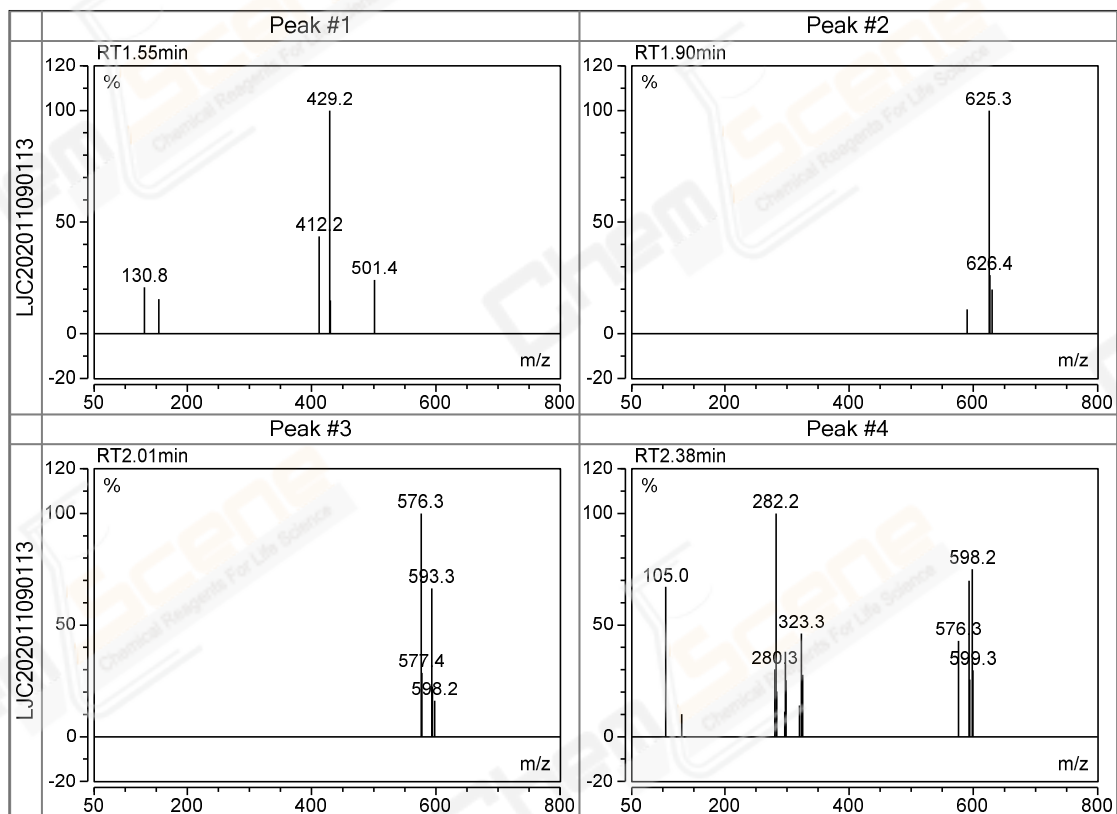

components_1

Mass	Intensity	Relative Intensity
m/z	counts	%
429.20	656944	100.00%

components_2

Mass	Intensity	Relative Intensity
m/z	counts	%
625.31	14967054	100.00%

components_3

Mass	Intensity	Relative Intensity
m/z	counts	%
576.30	91883484	100.00%

components_4

Mass	Intensity	Relative Intensity
m/z	counts	%
282.24	1193840	100.00%