



File ..\DATA\2021\20210208\1275\BIZ2021-208-SCH2.D Tgt Mass (CHM):
 Injection Date : 8 Feb 21 4:59 pm +0800 Seq. Line : 88
 Sample Name : BIZ2021-208-SCH2 Location : P1-B-02
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210208\1275\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210208\1275\1-POS-3MIN.M
 CAS NO. : 2114651-20-4
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

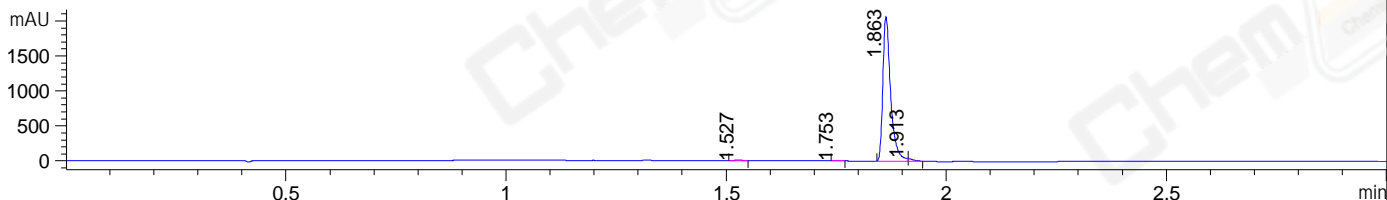


DAD1 C, Sig=254,4 Ref=off

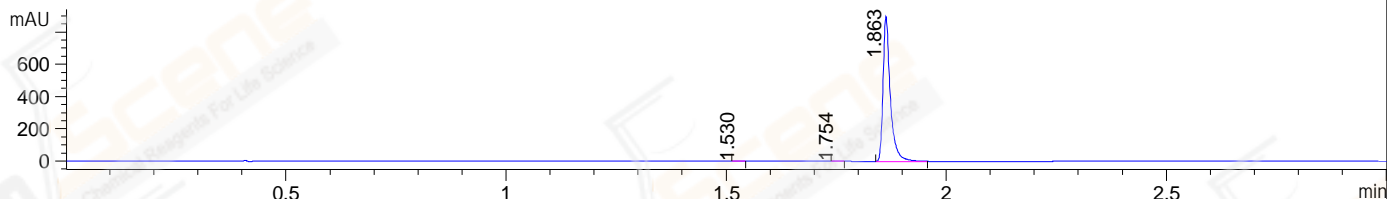

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

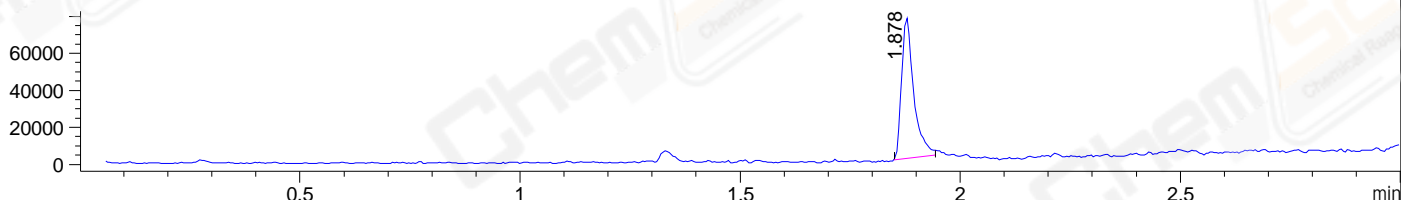

Ion 209, MSD1 209, Target Mass 208 +H Positive, EIC=208.7:209.7

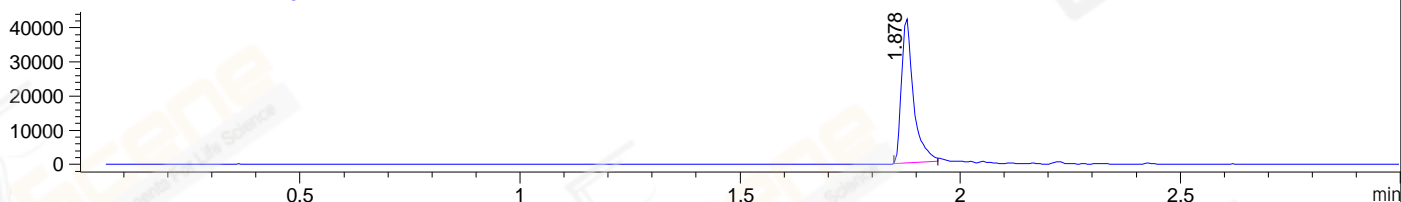

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.53	0.02	6.56	5.31	0.25	ND
1.75	0.01	2.36	2.64	0.09	ND
1.86	0.02	2537.98	2067.52	98.59	209
1.91	0.01	27.45	37.99	1.07	209

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.53	0.02	0.96	1.01	0.09	ND
1.75	0.01	0.84	0.96	0.08	ND
1.86	0.02	1033.73	899.91	99.83	209

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.88	0.03	147083.33	75999.20	100.00	209

Ret. Time: 1.88

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

