



File ..DATA\2021\20210310\1299\BIZ2021-308-WLQ16.D Tgt Mass (CHM):
 Injection Date : 10 Mar 21 7:21 pm +0800 Seq. Line : 127
 Sample Name : BIZ2021-308-WLQ16 Location : P1-B-03
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210310\1299\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210310\1299\1-POS-3MIN.M
 Product Name: BIM-23190 (hydrochloride)
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

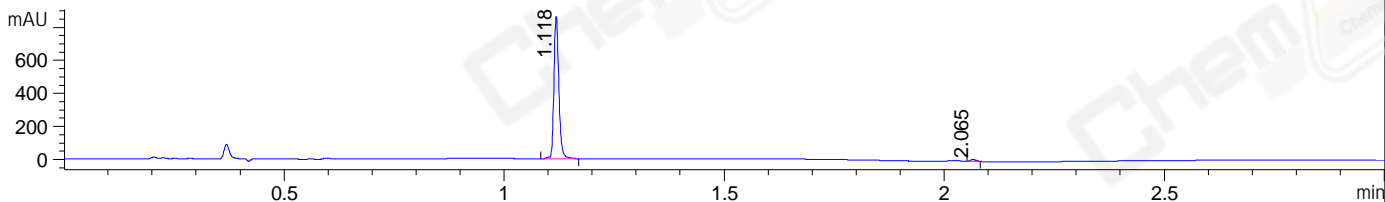


DAD1 C, Sig=254,4 Ref=off

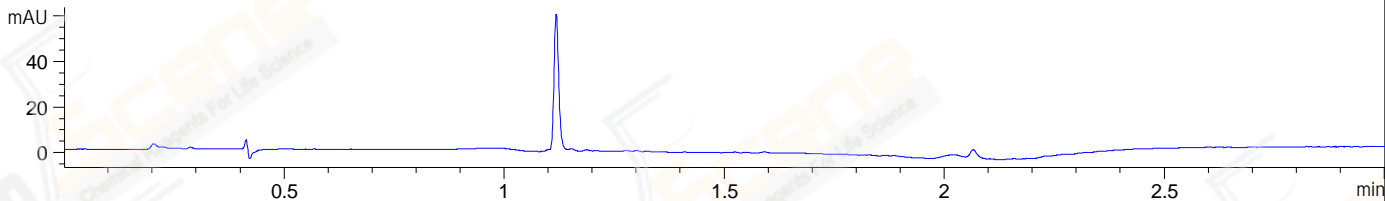

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

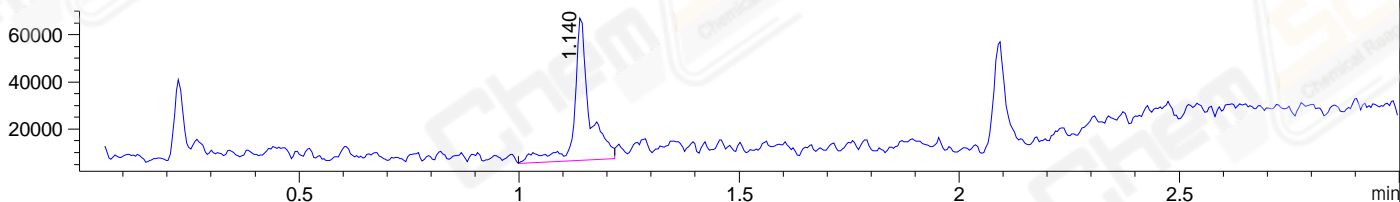

Ion 1202, MSD1 1202, Target Mass 1201 +H Positive, EIC=1201.7:1202.7

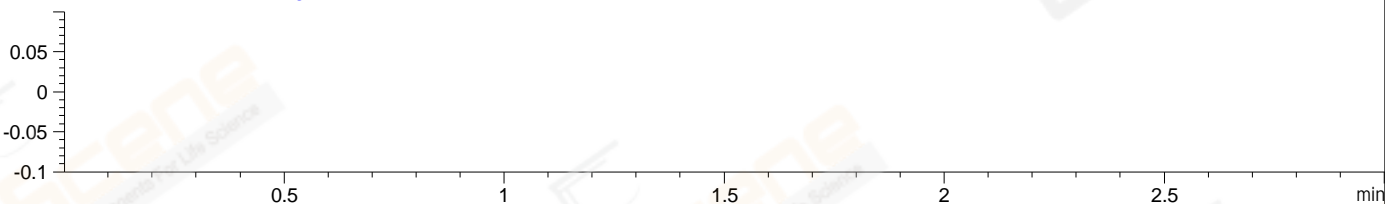

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.12	0.01	671.61	865.21	98.62	602
2.07	0.02	9.38	10.23	1.38	345

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
--------	-------	------	--------	-------	-------

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.14	0.03	146821.70	60969.90	100.00	602

Ret. Time: 1.14

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

