



File ..\DATA\2021\20210315\1305\BIZ2021-315-WMX3.D Tgt Mass (CHM):
 Injection Date : 15 Mar 21 7:26 pm +0800 Seq. Line : 130
 Sample Name : BIZ2021-315-WMX3 Location : P1-D-08
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210315\1305\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210315\1305\1-POS-3MIN.M
 CAS NO. : 10179-57-4
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

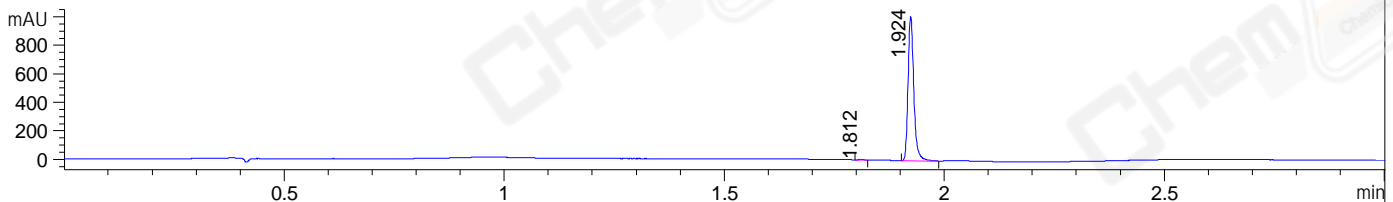


DAD1 C, Sig=254,4 Ref=off

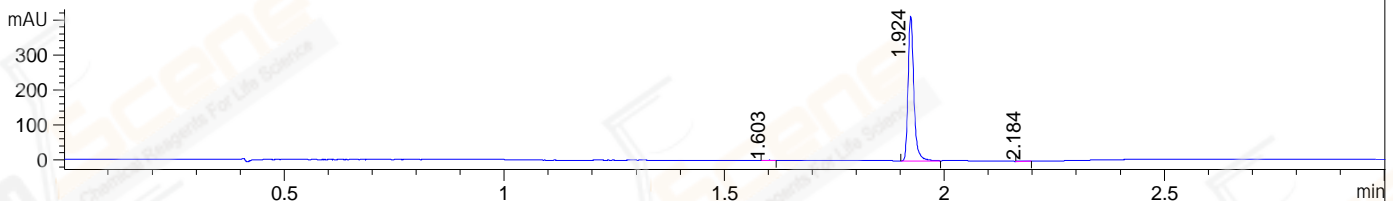

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

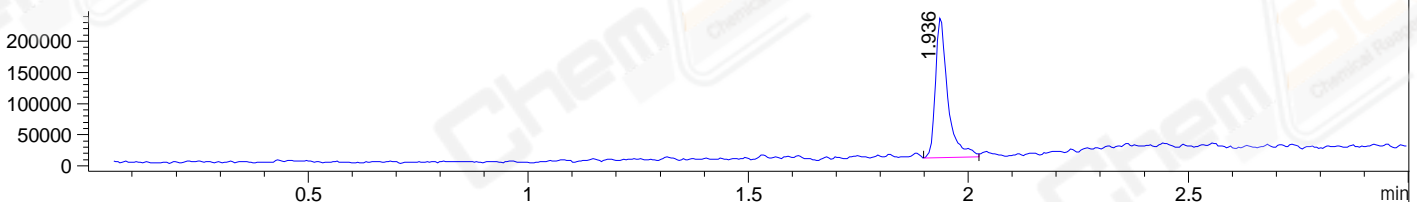

Ion 378, MSD1 378, Target Mass 377 +H Positive, EIC=377.7:378.7

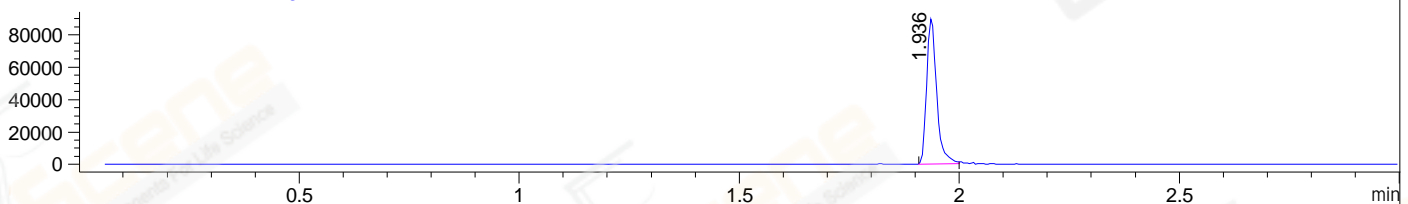

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.81	0.01	2.37	2.76	0.26	ND
1.92	0.02	917.83	1013.17	99.74	378

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.60	0.02	0.42	0.39	0.11	ND
1.92	0.02	375.54	414.08	99.73	378
2.18	0.01	0.61	0.72	0.16	305

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.94	0.03	444218.25	226471.38	100.00	378

Ret. Time: 1.94

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

