
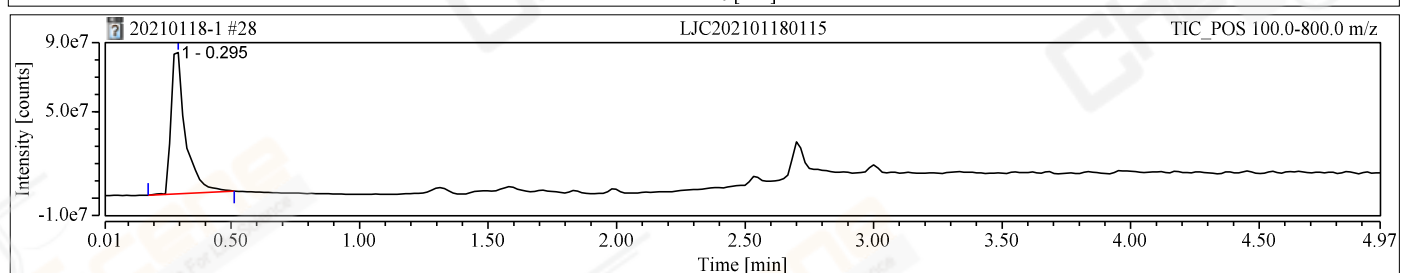
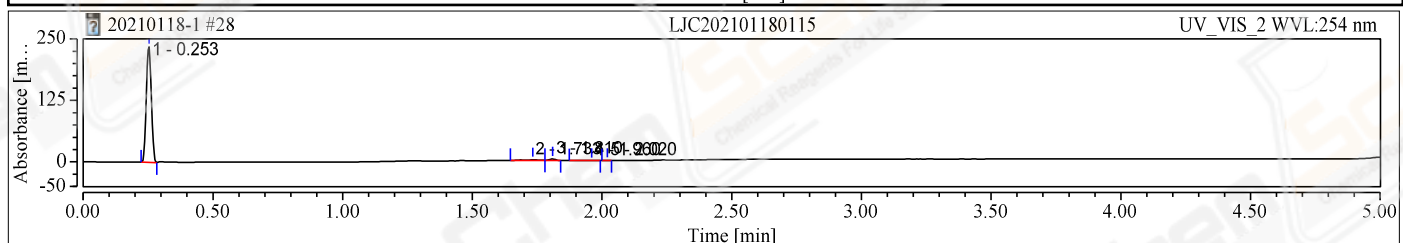


## Chromatogram and Results

Injection Name: LJC202101180115	Channel: TIC_POS
Vial Number: RC8	Wavelength: 220.0
Injection Type: Unknown	Injection Volume: 1.00
Calibration Level: AHM003	Injection Time: 18/01/2021 16:40
Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0	InstMeth.creation_time: 28/08/2020 09:10
Processing Method: LJC202101180115	Last update_time: 18/Jan/2021 16:53
seq.creation_operator: Mbaogd	Data Operator: Mbaogd
CAS NO.: 1477-68-5	
chrom: TIC_POS.chm	

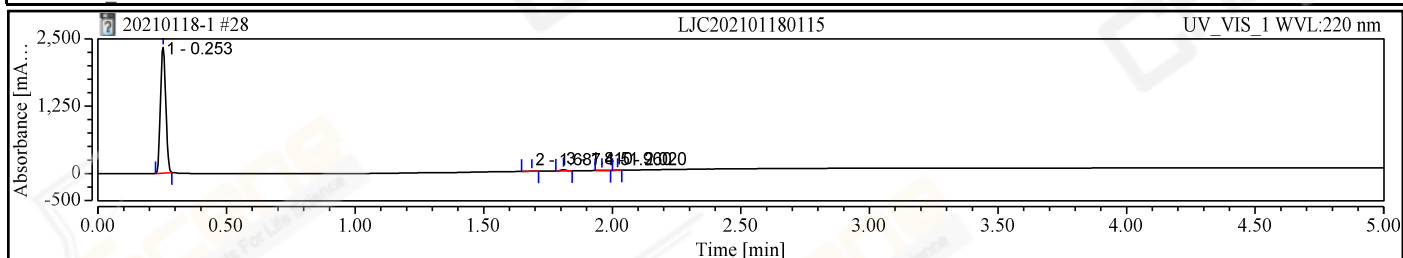


### Peak Results for UV\_VIS\_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	0.253	55.593	2333.978	687	34.19	1.06	98.82	
2	1.687	0.071	2.469	22285	2.96	0.88	0.13	
3	1.810	0.573	24.101	35800	3.55	1.01	1.02	
4	1.960	0.007	0.253	28661	n.a.	1.20	0.01	
5	2.020	0.013	0.677	n.a.	n.a.	0.97	0.02	
<b>Total:</b>		56.257	2361.477	87433.000	40.69			

### Peak Results for UV\_VIS\_2

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	0.253	5.348	235.016	752	33.86	1.02	97.12	
2	1.733	0.068	1.272	18866	1.71	0.77	1.23	
3	1.810	0.076	3.130	34453	3.51	0.99	1.38	
4	1.960	0.009	0.166	28443	n.a.	0.69	0.16	
5	2.020	0.007	0.344	n.a.	n.a.	0.97	0.12	
<b>Total:</b>		5.507	239.929	82514.000	39.08			

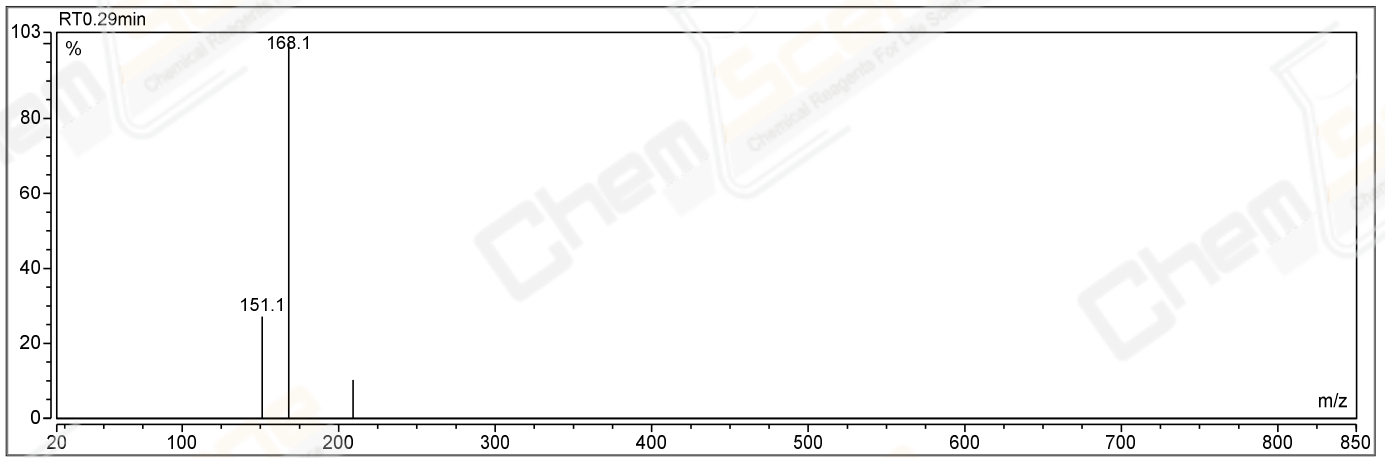

components\_1

Mass	Intensity	Relative Intensity
m/z	counts	%
168.13	52971607	100.00%