
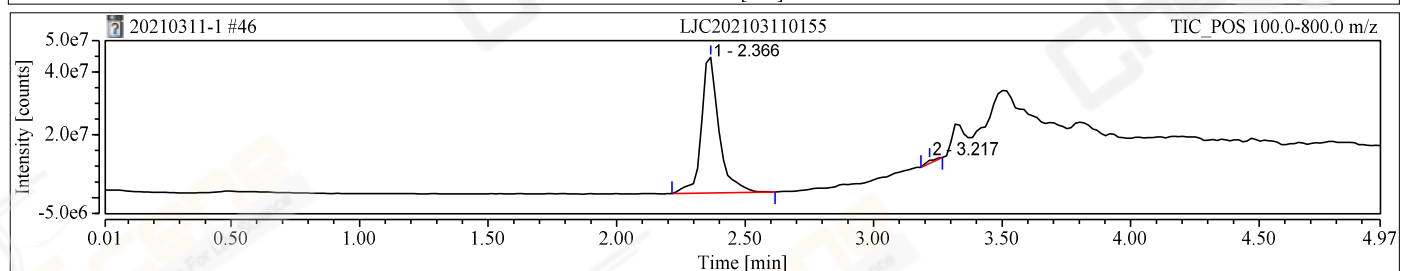
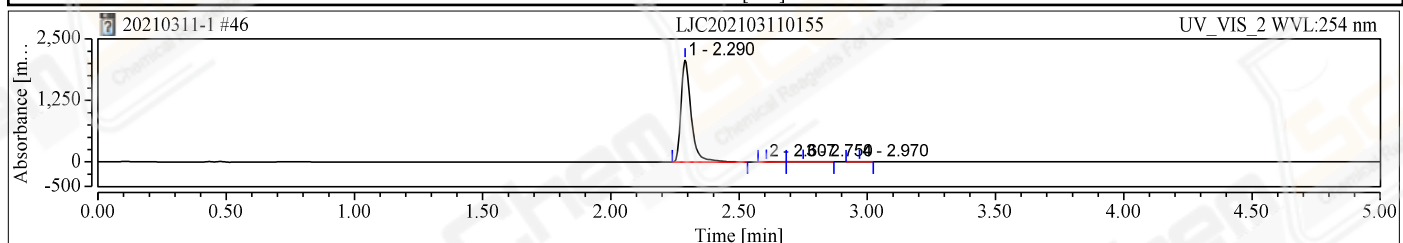


Chromatogram and Results

Injection Name: LJC202103110155	Channel: TIC_POS
Vial Number: RA4	Wavelength: 220.0
Injection Type: Unknown	Injection Volume: 1.00
Calibration Level: AHM003	Injection Time: 11/03/2021 18:38
Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0	InstMeth.creation_time: 28/08/2020 09:10
Processing Method: LJC202103110155	Last update_time: 12/Mar/2021 09:23
seq.creation_operator: Mbaogd	Data Operator: Mbaogd
CAS NO.: 501-36-0 228.24	Print Operator: Mbaogd
chrom: TIC_POS.chm	

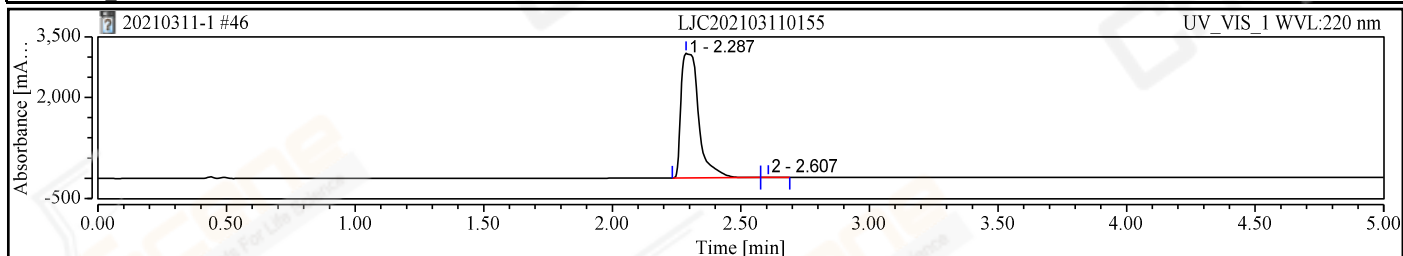


Peak Results for UV_VIS_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	2.287	244.903	3083.938	8588	3.93	2.33	99.90	
2	2.607	0.253	5.728	26281	n.a.	1.88	0.10	
Total:		245.156	3089.666	34869.000	3.93			

Peak Results for UV_VIS_2

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	2.290	93.691	2070.755	18671	5.04	1.45	99.78	
2	2.607	0.125	3.174	31607	1.16	1.74	0.13	
3	2.750	0.050	0.471	3437	1.88	1.39	0.05	
4	2.970	0.027	1.037	66168	n.a.	1.30	0.03	
Total:		93.893	2075.437	119883.000	8.08			

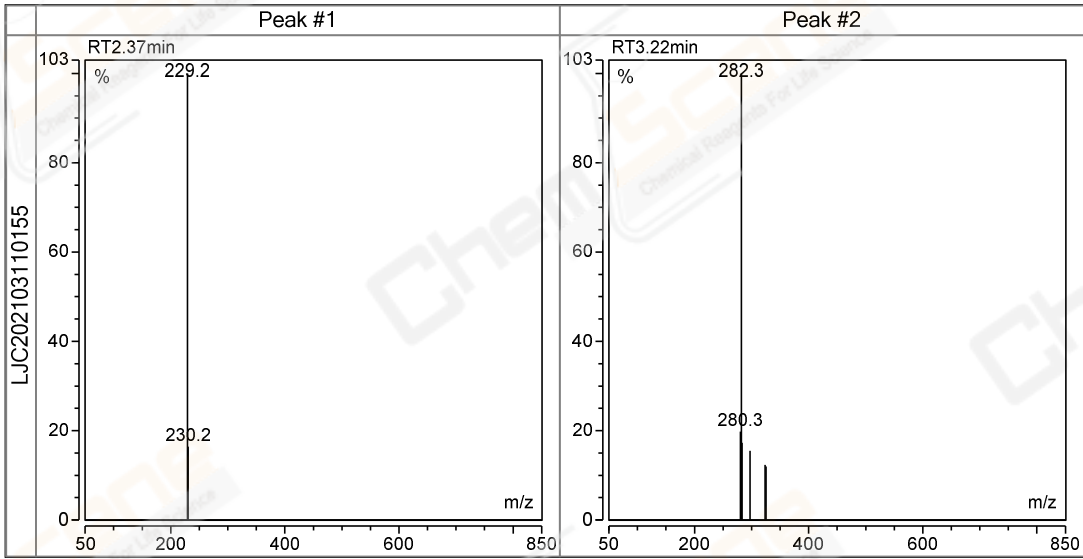

components_1

Mass	Intensity	Relative Intensity
m/z	counts	%
229.17	31506232	100.00%

components_2

Mass	Intensity	Relative Intensity
m/z	counts	%
282.33	3640567	100.00%