
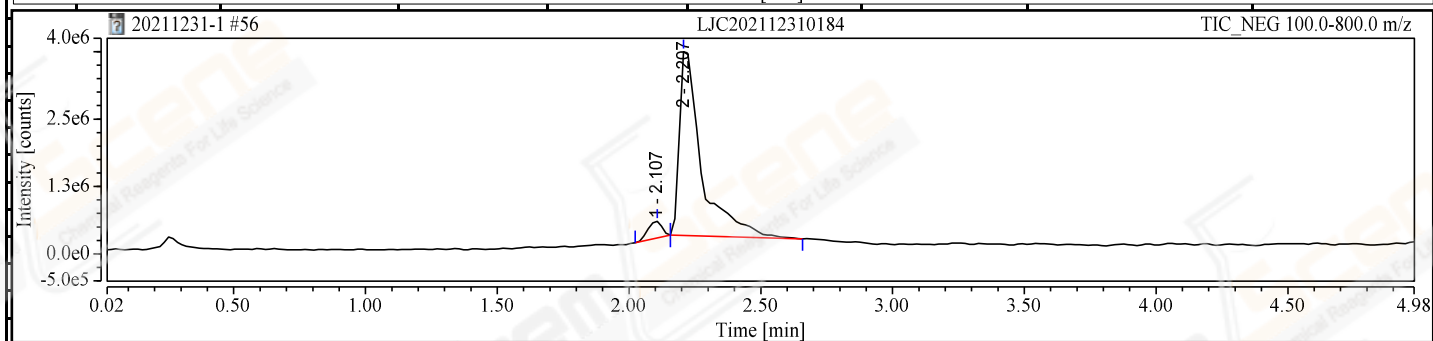
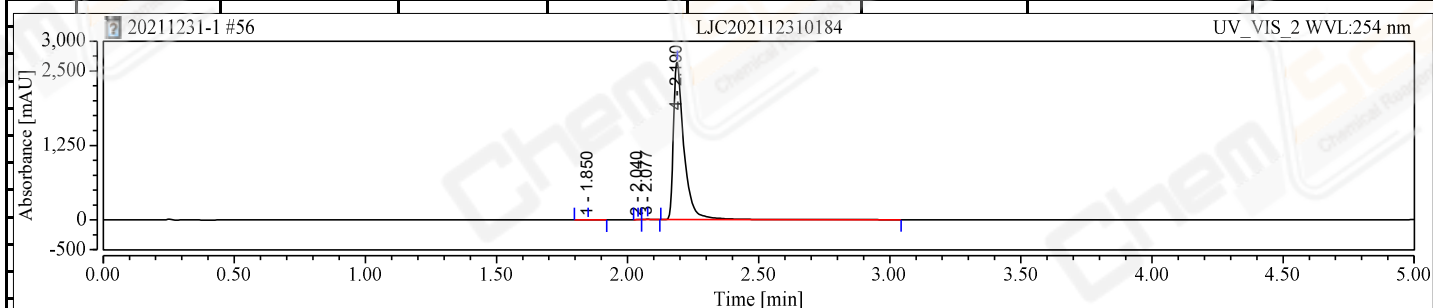


## Chromatogram and Results

Injection Name: LJC202112310184	Channel: TIC_NEG
Vial Number: BC3	Wavelength: 220
Injection Type: Unknown	Injection Volume: 1
Calibration Level: AHM003	Injection Time: 31/12/2021 17:34
Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0	InstMeth.creation_time: 28/08/2020 09:10
Processing Method: LJC202112310184	Last update_time: 04/01/2022 09:59
seq.creation_operator Mliy	Data Operator: Mliy
CAS NO.: 1135616-49-7	Print Operator: Mliy
chrom://ahyy-cm7/CM7DATA/1-RND/LCMS/AHM003/Sequence/2021/202112/20211231-1.seq/691.smp/UV_VIS_1.channel/UV_VIS_1.chm	

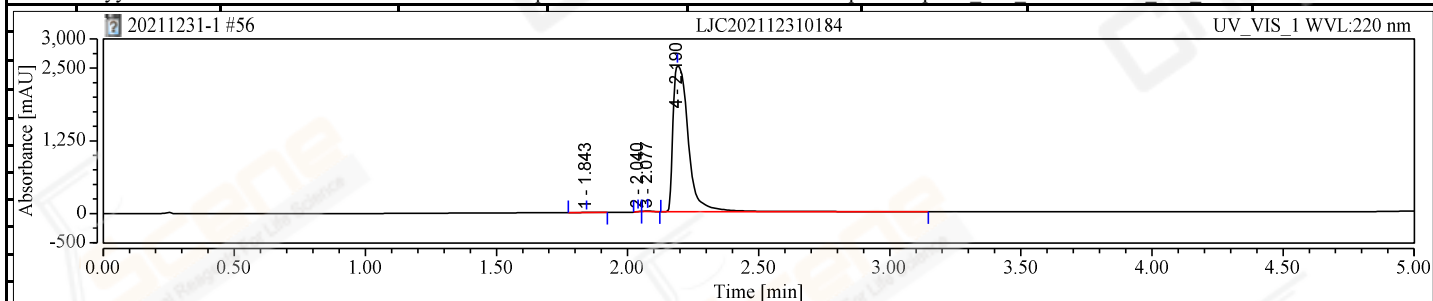



### Peak Results for UV\_VIS\_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	1.843	0.046	0.770	5465	2.30	1.47	0.027	
2	2.040	0.043	2.786	13084	0.60	0.99	0.025	
3	2.077	0.352	11.292	26810	1.58	1.36	0.205	
4	2.190	170.849	2511.037	8903	n.a.	2.20	99.742	
<b>Total:</b>		171.289671	2525.885542	54262	4.48			

### Peak Results for UV\_VIS\_2

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Match	Rel.Area %	Peak Name
1	1.850	0.012	0.198	6464	2.20	n.a.	0.009	
2	2.040	0.013	0.855	10253	0.55	n.a.	0.011	
3	2.077	0.128	3.916	24054	1.91	n.a.	0.104	

4	2.190	123.241	2635.407	17962	n.a.	n.a.	99.876	
Total:		123.3937231	2640.375357	58733	4.65			

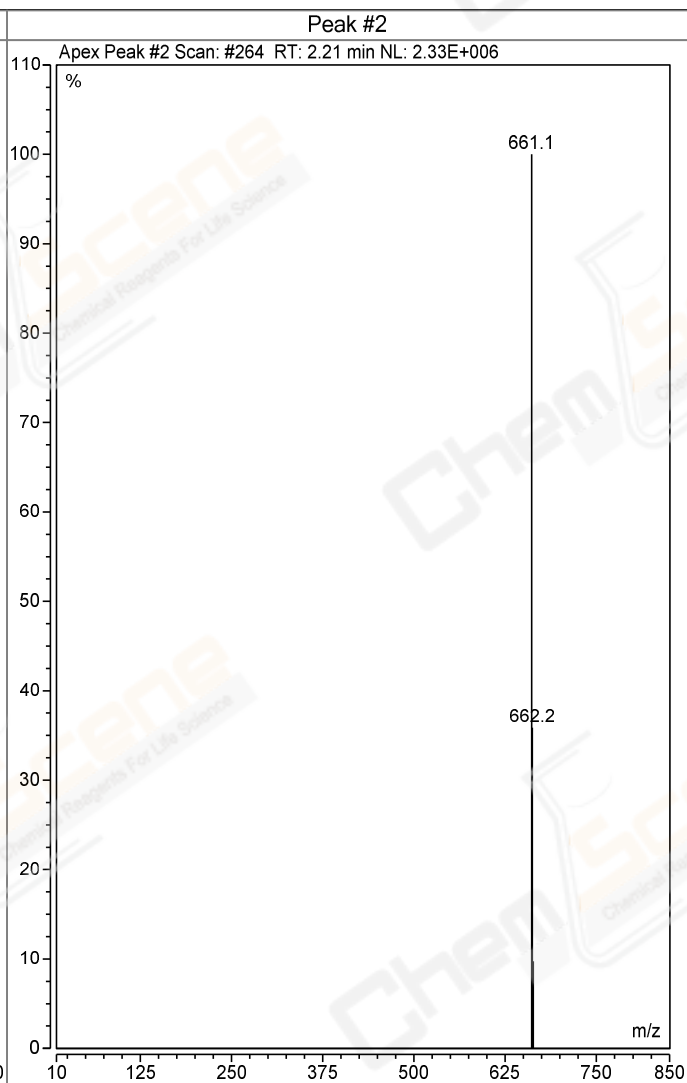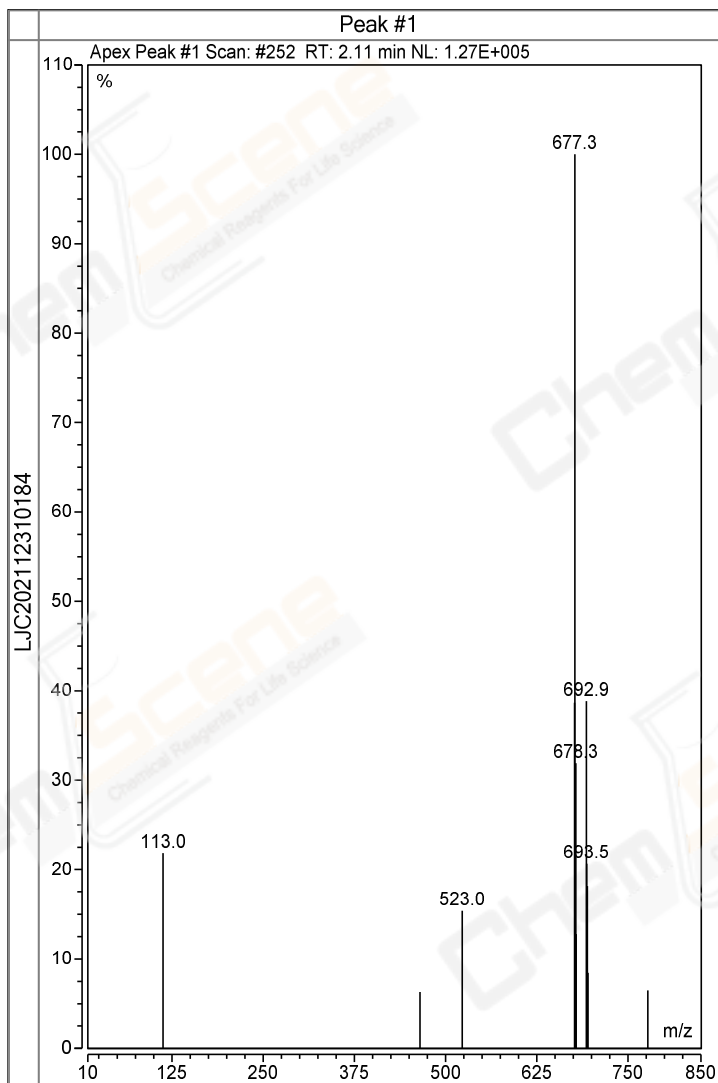

**components\_1**

Mass	Intensity	Relative Intensity
m/z	counts	%
677.31	127302	100.00%

**components\_2**

Mass	Intensity	Relative Intensity
m/z	counts	%
661.08	2331269	100.00%