
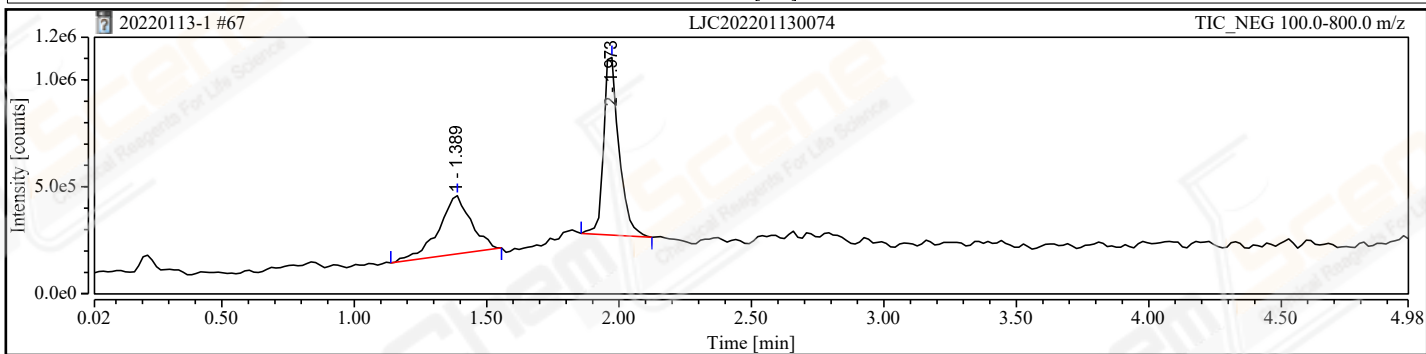
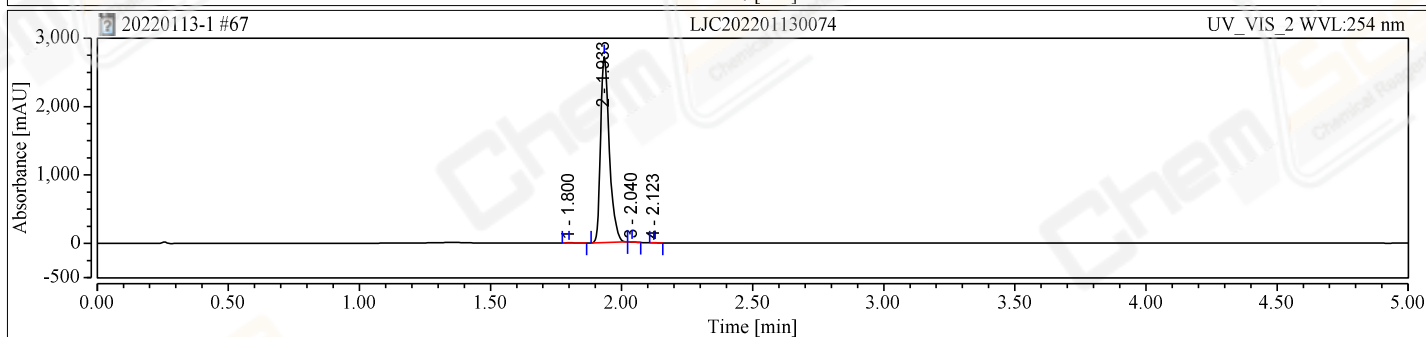


Chromatogram and Results

Injection Name: LJC202201130074 Vial Number: RB5 Injection Type: Unknown Calibration Level: AHM003 Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0 Processing Method: LJC202201130074 seq.creation_operator: mlih CAS NO.: 3029-64-9	Channel: TIC_NEG Wavelength: 220 Injection Volume: 1 Injection Time: 13/01/2022 16:15 InstMeth.creation_time: 28/08/2020 09:10 Last update_time: 13/01/2022 16:44 Data Operator: mlih Print Operator: mlih
---	---

chrom://ahyy-cm7/CM7DATA/1-RND/LCMS/AHM003/Sequence/2022/202201/20220113-1.seq/669.smp/UV_VIS_1.channel/UV_VIS_1.chm

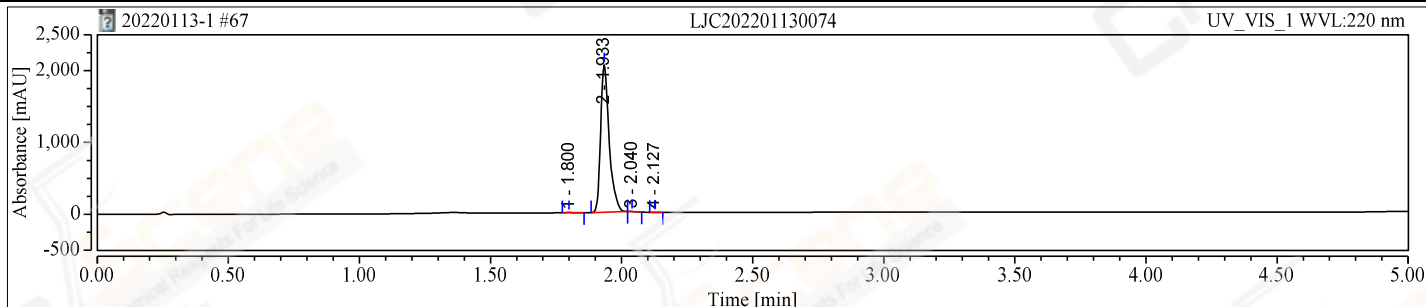



Peak Results for UV_VIS_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	1.800	0.055	1.847	23356	2.57	1.44	0.071	
2	1.933	77.349	2051.981	18710	1.91	1.44	99.845	
3	2.040	0.047	2.091	21724	1.88	1.23	0.061	
4	2.127	0.018	0.773	52900	n.a.	1.25	0.023	
Total:		77.46889915	2056.691677	116690	6.36			

Peak Results for UV_VIS_2

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Match	Rel.Area %	Peak Name
1	1.800	0.108	3.100	18200	2.38	n.a.	0.103	
2	1.933	105.070	2715.633	17410	1.85	n.a.	99.834	

3	2.040	0.038	1.606	20573	1.75	n.a.	0.036	
4	2.123	0.029	1.141	48454	n.a.	n.a.	0.027	
Total:		105.2453869	2721.47958	104637	5.97			

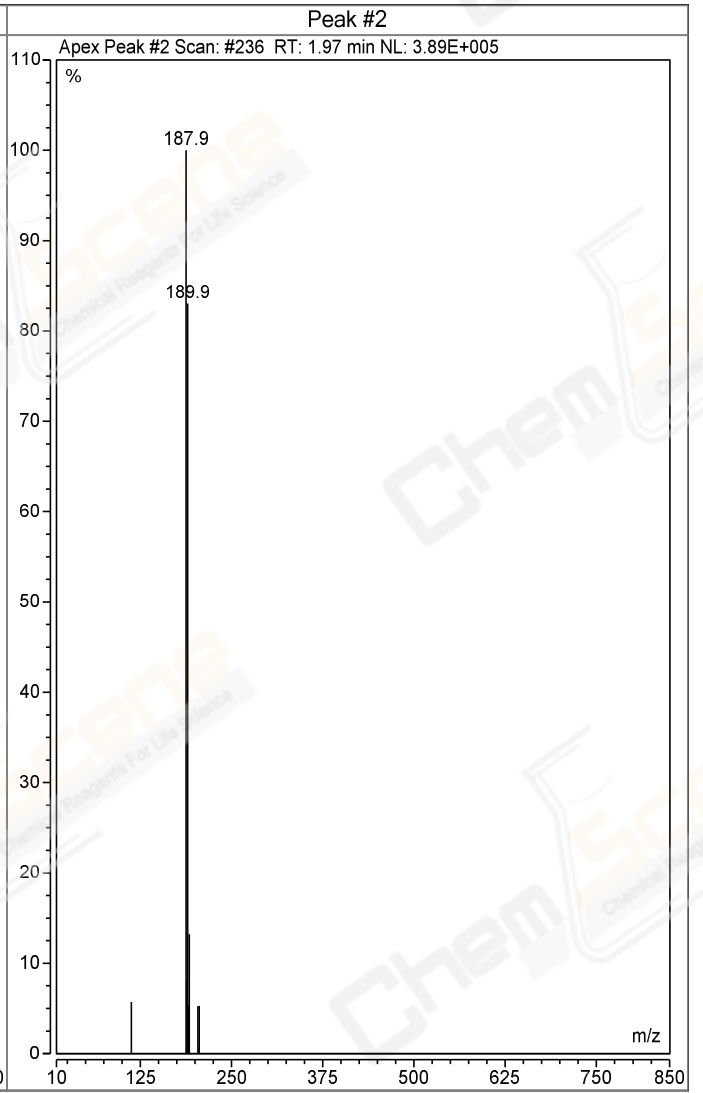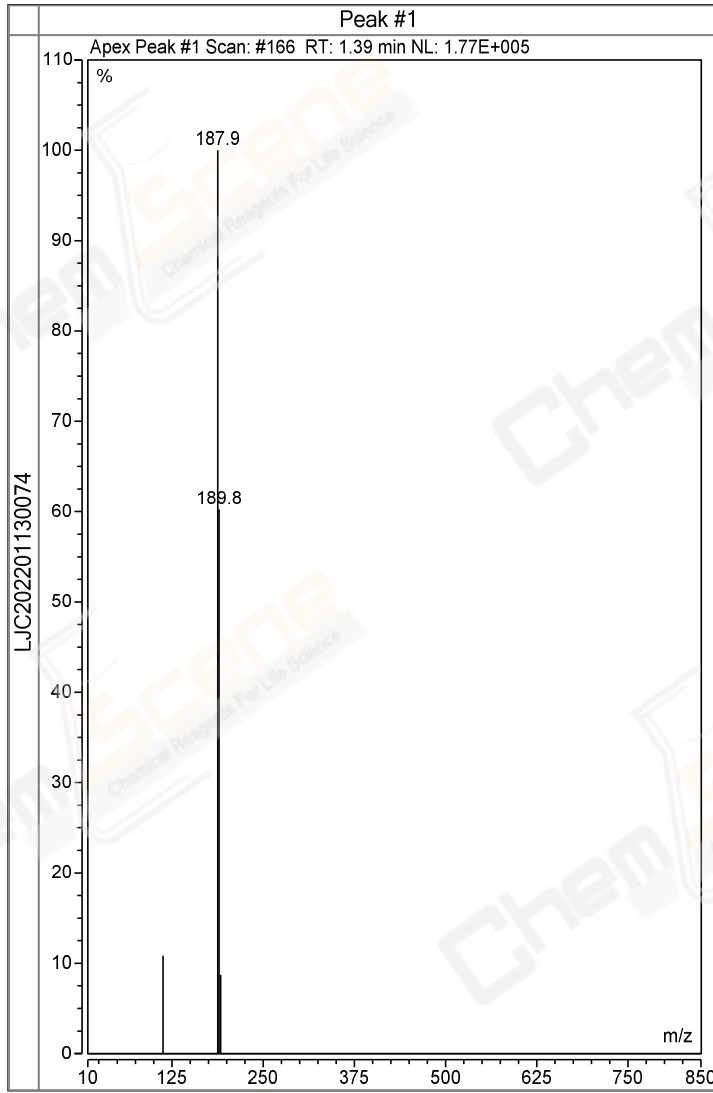

components_1

Mass	Intensity	Relative Intensity
m/z	counts	%
187.87	176837	100.00%

components_2

Mass	Intensity	Relative Intensity
m/z	counts	%
187.92	389335	100.00%