
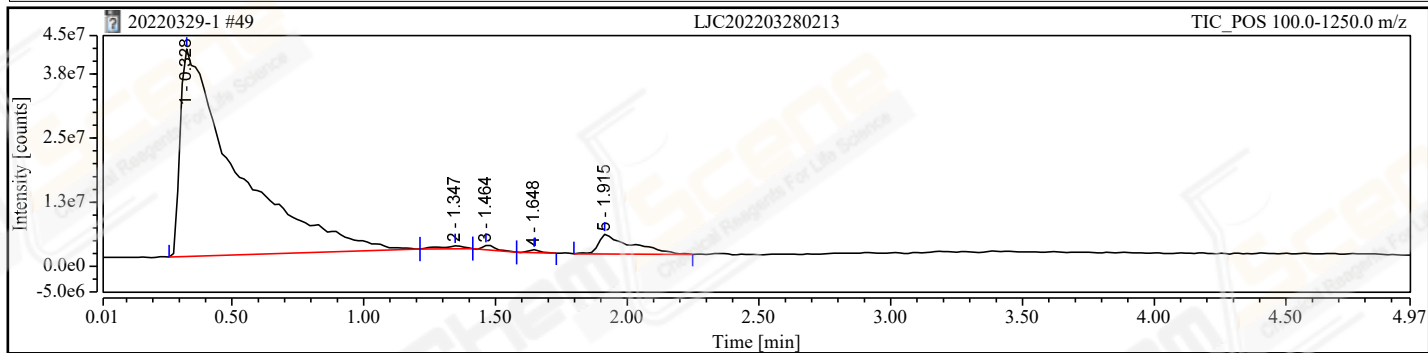
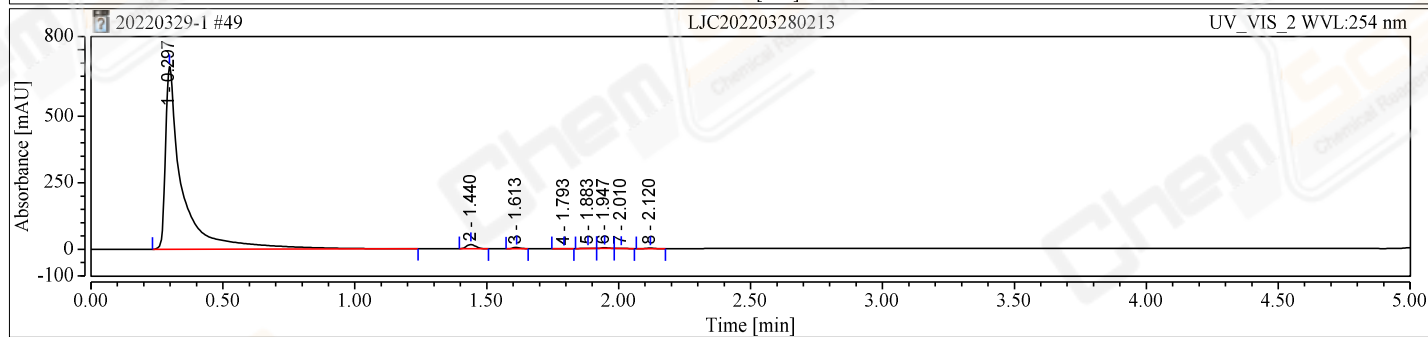


Chromatogram and Results

Injection Name: LJC202203280213	Channel: TIC_POS
Vial Number: GA6	Wavelength: 220
Injection Type: Unknown	Injection Volume: 1
Calibration Level: AHM003	Injection Time: 29/03/2022 13:23
Instrument Method: LCMS-1.0-5min	InstMeth.creation_time: 28/08/2020 09:10
Processing Method: LJC202203280213	Last update_time: 30/03/2022 10:18
seq.creation_operator: mlih	Data Operator: mlih
CAS NO.: 884507-17-9	Print Operator: mlih


chrom://ahyy-cm7/CM7DATA/1-RND/LCMS/AHM003/Sequence/2022/202203/20220329-1.seq/785.smp/UV_VIS_1.channel/UV_VIS_1.chm

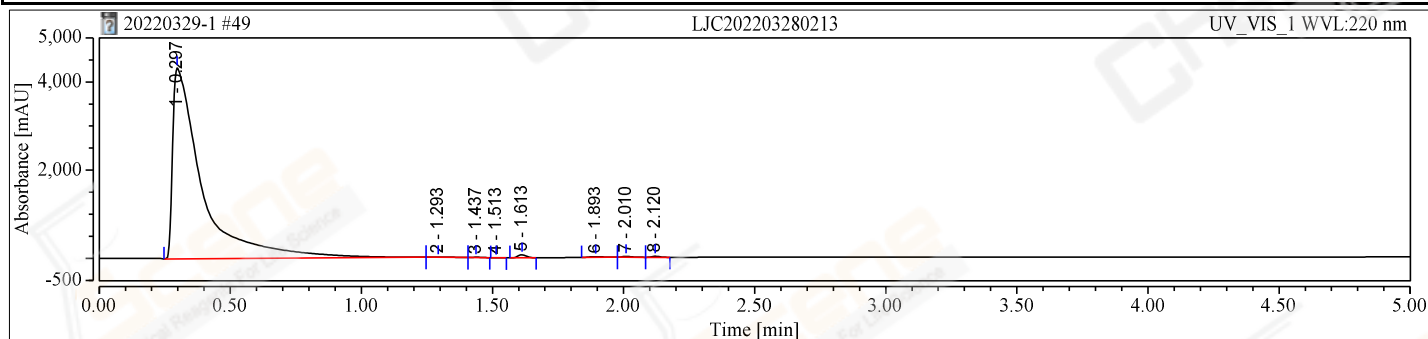

Peak Results for UV_VIS_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Match	Rel.Area %	Peak Name
1	0.297	561.783	4323.762	51	6.22	n.a.	99.034	
2	1.293	0.219	1.489	1124	1.31	n.a.	0.039	
3	1.437	0.263	6.573	7930	1.37	n.a.	0.046	
4	1.513	0.027	0.837	16321	1.87	n.a.	0.005	
5	1.613	2.424	65.584	11688	3.51	n.a.	0.427	
6	1.893	1.001	15.776	5760	1.46	n.a.	0.176	
7	2.010	0.730	19.363	17934	1.85	n.a.	0.129	
8	2.120	0.819	22.518	20562	n.a.	n.a.	0.144	
Total:		567.266	4455.902	81370	17.58			

Peak Results for UV_VIS 2								
No.	Retention Time	Area	Height	Plates (USP)	Resolution (USP)	Match	Rel.Area	Peak Name
	min	mAU*min	mAU				%	
1	0.297	50.466	687.102	258	16.60	n.a.	97.903	
2	1.440	0.623	15.827	8148	2.82	n.a.	1.210	
3	1.613	0.176	4.838	11896	2.92	n.a.	0.341	
4	1.793	0.023	0.583	12557	1.33	n.a.	0.045	
5	1.883	0.048	1.024	11249	1.01	n.a.	0.093	
6	1.947	0.096	2.926	20652	1.17	n.a.	0.186	
7	2.010	0.037	1.104	22149	1.92	n.a.	0.071	
8	2.120	0.078	2.062	19630	n.a.	n.a.	0.152	
Total:		51.547	715.466	106539	27.78			

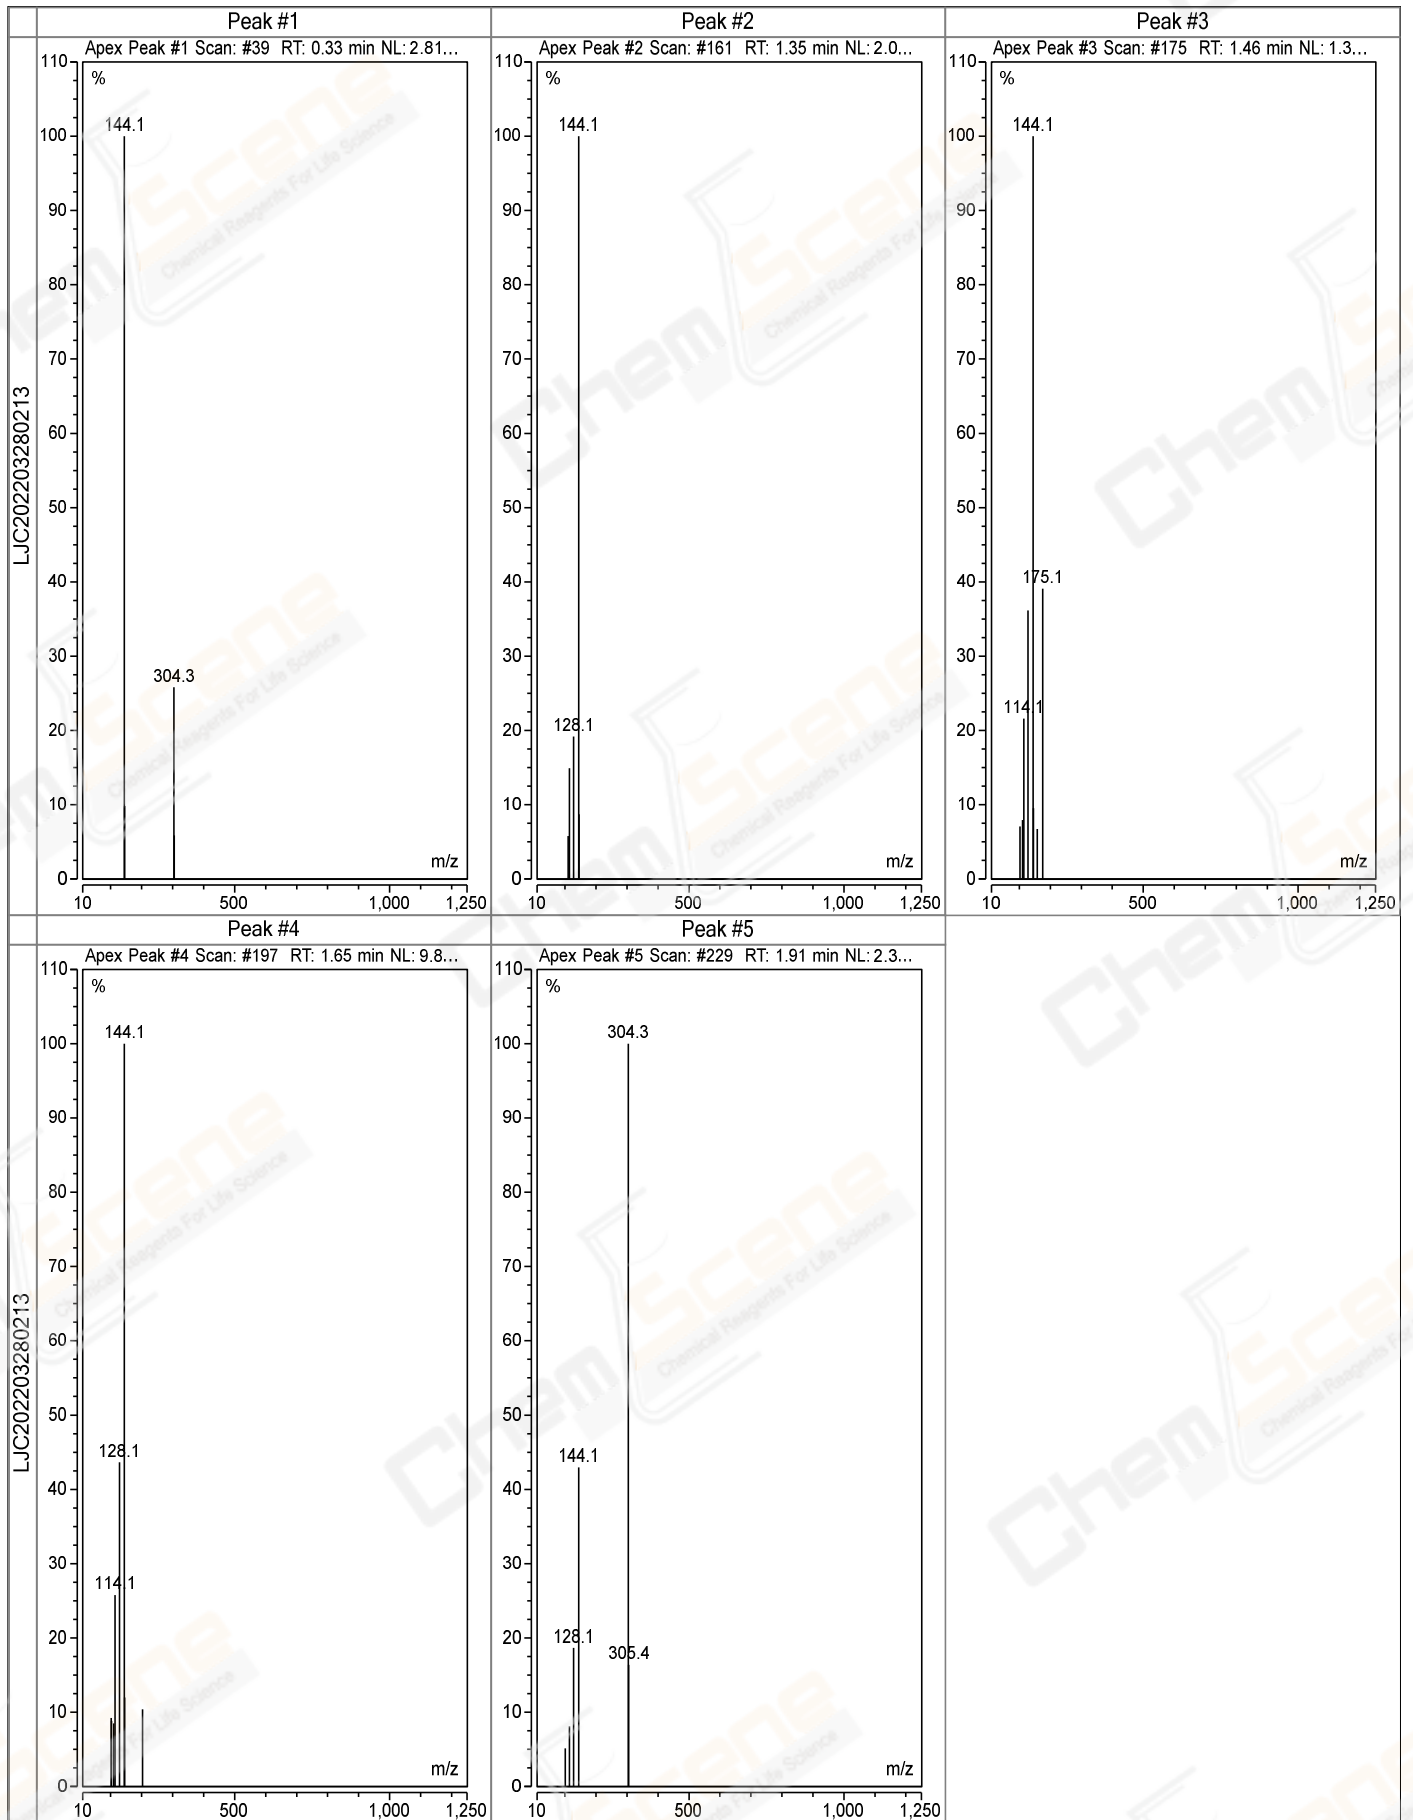

components_1	Mass	Intensity	Relative Intensity
	m/z	counts	%
	144.09	28075500	100.00%
components_2	Mass	Intensity	Relative Intensity
	m/z	counts	%
	144.08	2090479	100.00%
components_3	Mass	Intensity	Relative Intensity
	m/z	counts	%
	144.11	1365140	100.00%
components_4	Mass	Intensity	Relative Intensity
	m/z	counts	%
	144.10	988198	100.00%
components_5	Mass	Intensity	Relative Intensity
	m/z	counts	%
	304.25	2388219	100.00%