
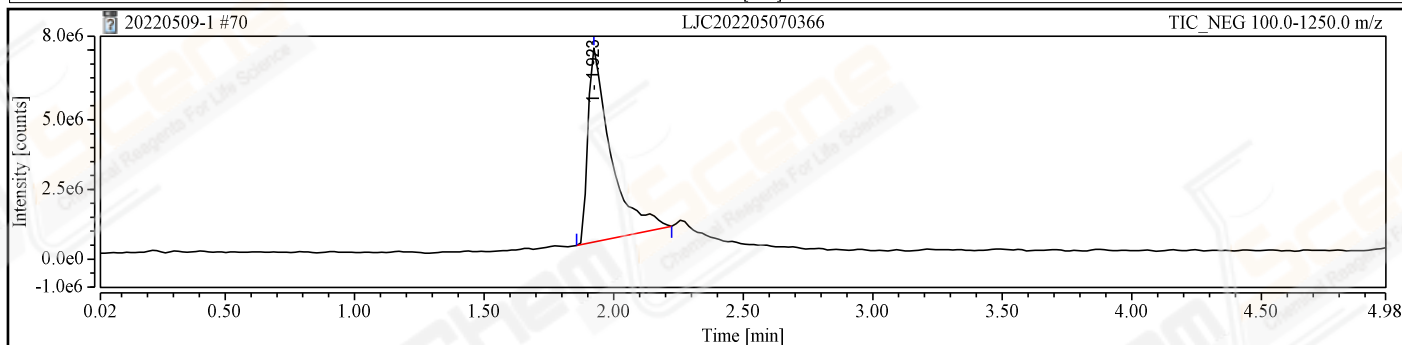
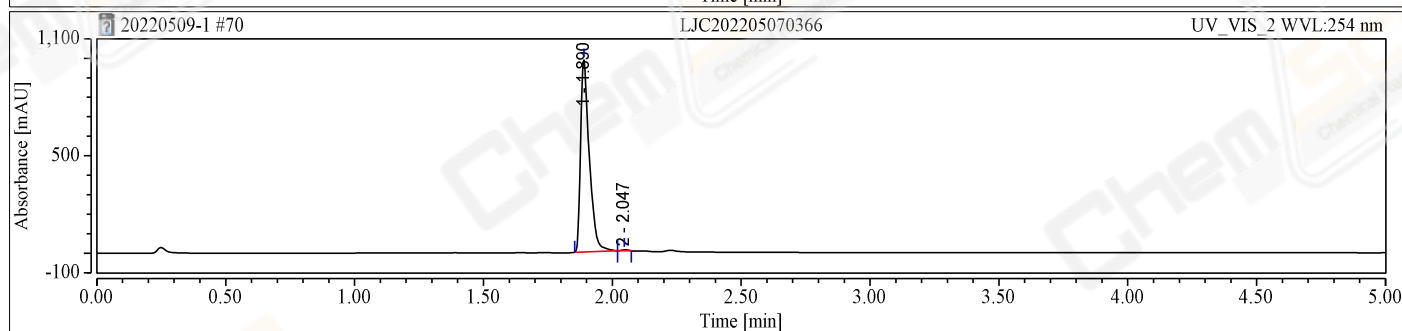


Chromatogram and Results

Sample ID:	LJC202205070366	Comment:	221.05
Batch No.:		Channel:	TIC_NEG
Vial Number:	BA7	Wavelength:	220
Injection Type:	Unknown	Injection Volume:	1
Calibration Level:	LCMS10401	Injection Time:	09/05/2022 17:59
Instrument Method:	LCMS-1.0-5min	InstMeth.creation_time:	28/08/2020 09:10
Processing Method:	LJC202205070366	Last update_time:	10/05/2022 16:06
CAS NO.:	2173193-92-3		

chrom://ahyy-cm7/CM7DATA/ARD/LCMS/LCMS10401/Sequence/2022/202205/20220509-1.seq/685.smp/UV_VIS_1.channel/UV_VIS_1.chm

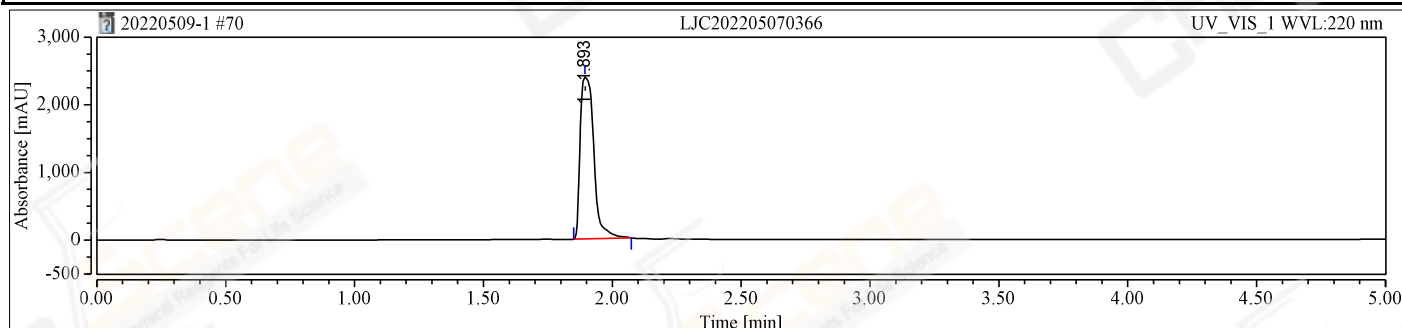


Peak Results for UV_VIS_1

No.	Retention Time	Area	Height	Plates (USP)	Resolution (USP)	Match	Rel.Area	Peak Name
	min	mAU*min	mAU				%	
1	1.893	146.632	2392.957	8557	n.a.	n.a.	100.000	
Total:		146.632	2392.957	8557	0.00			

Peak Results for UV_VIS_2

No.	Retention Time	Area	Height	Plates (USP)	Resolution (USP)	Match	Rel.Area	Peak Name
	min	mAU*min	mAU				%	
1	1.890	38.911	985.110	15744	2.98	n.a.	99.650	
2	2.047	0.137	5.087	33154	n.a.	n.a.	0.350	
Total:		39.048	990.197	48898	2.98			

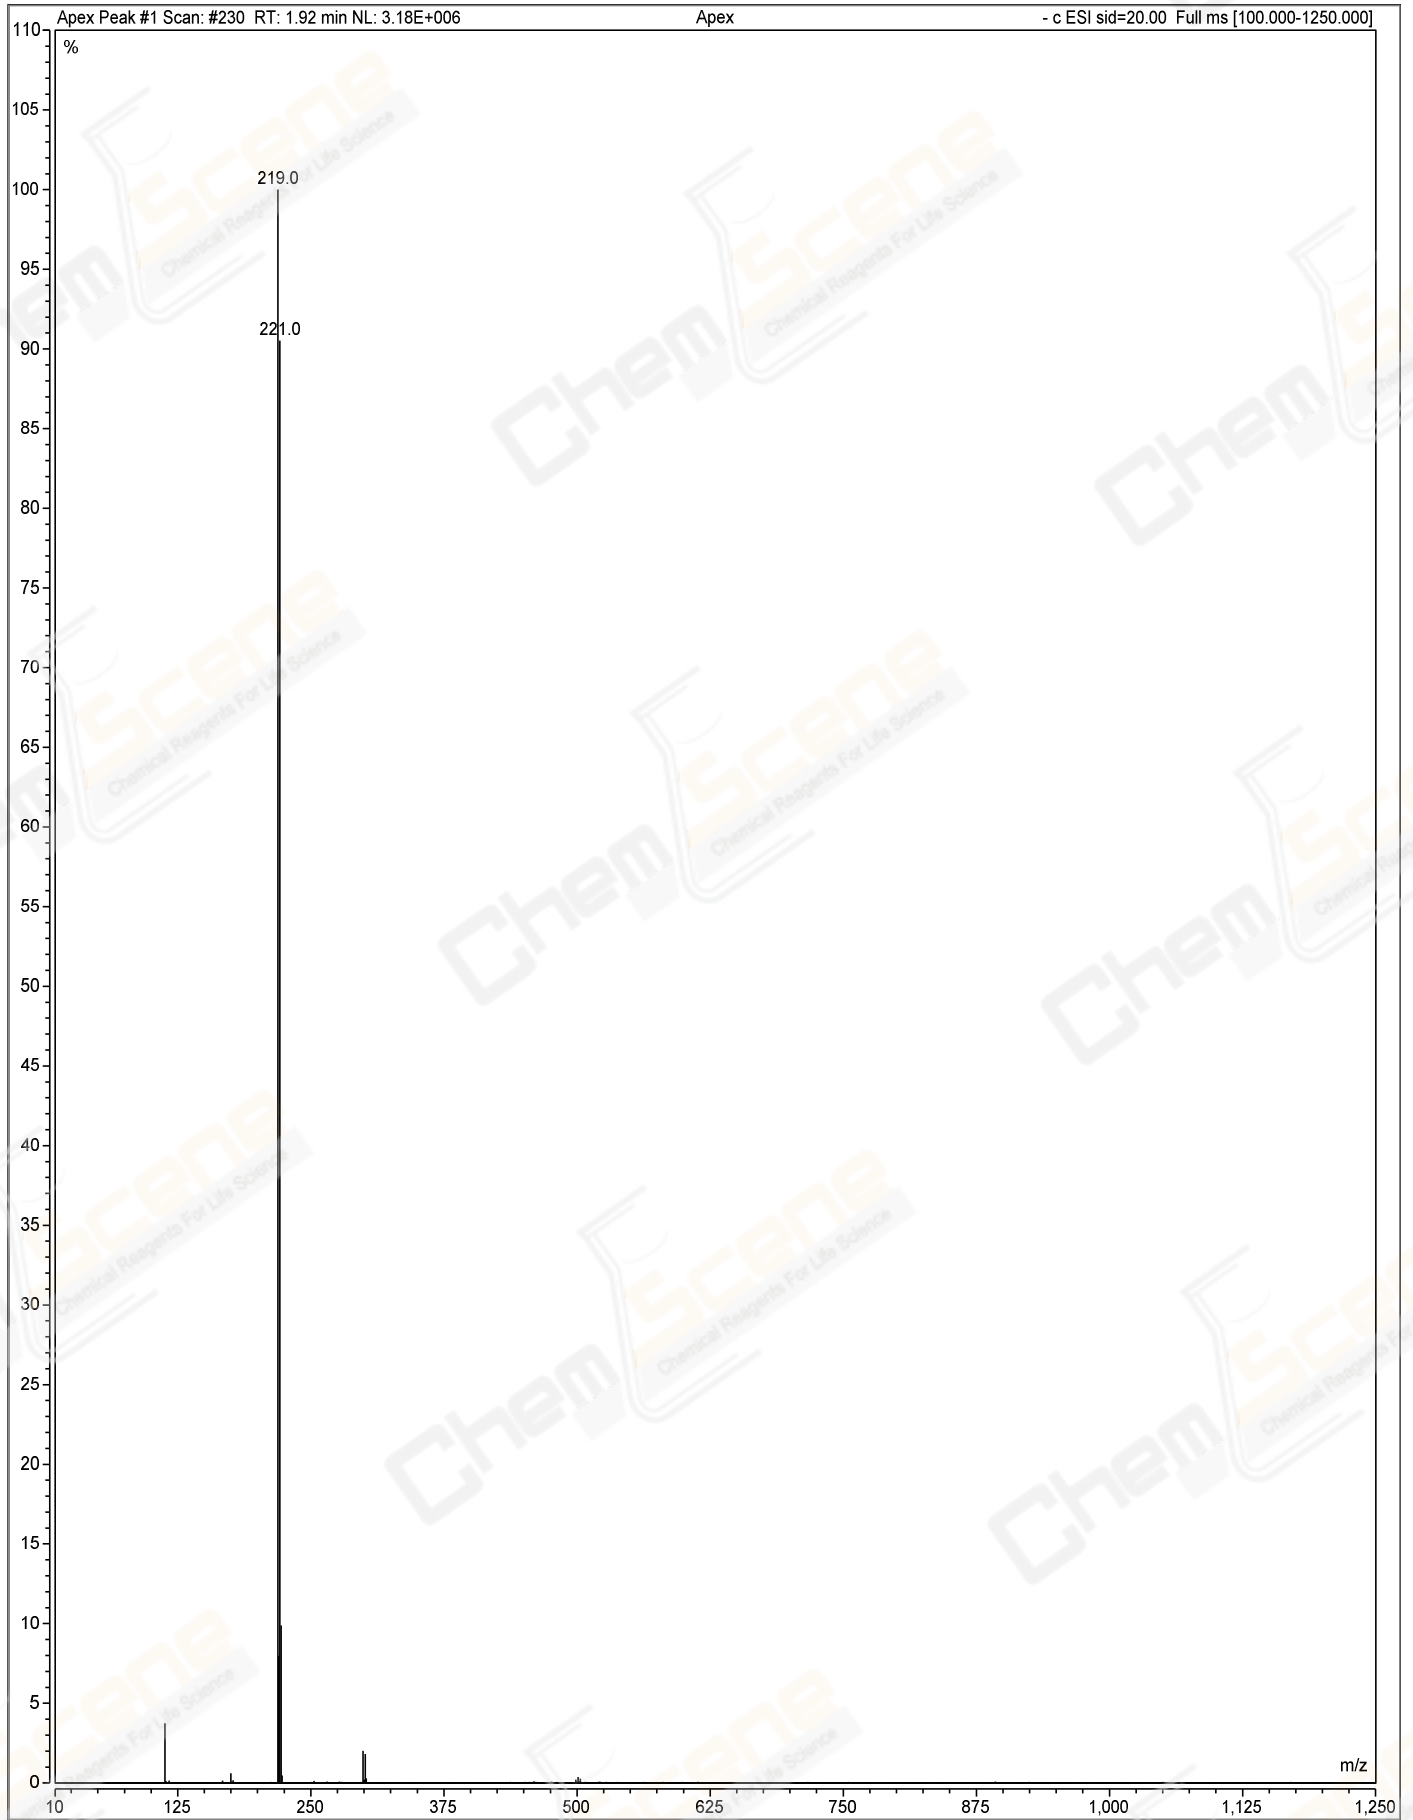

components_1

Mass	Intensity	Relative Intensity
m/z	counts	%
218.97	3183326	100.00%