


CAS NO.: 1362661-34-4

### MASS SPECTROMETRY REPORT

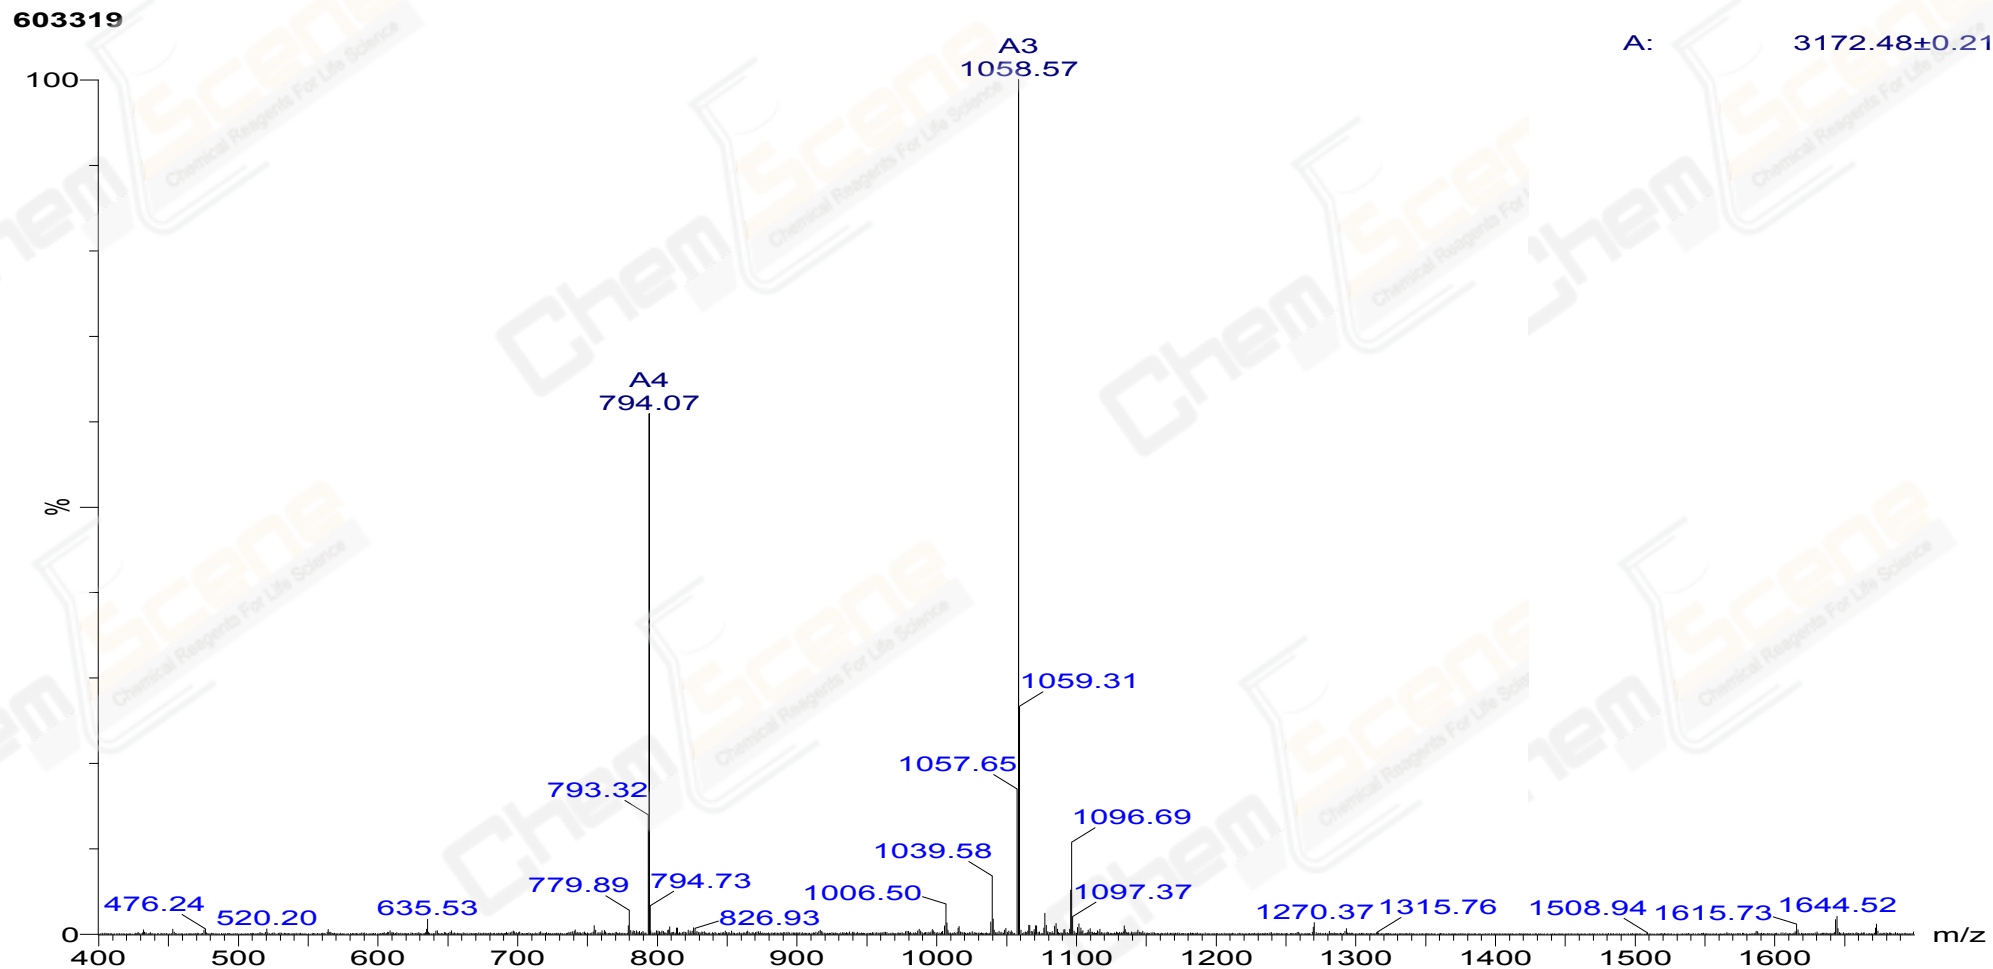

Sample Description

Analyzed date: 2021-12-20  
Analyst: SHAO  
Sample: 603319  
M.W.: 3173.6  
Lot. No.:

Instrument

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50%H2O/50%ACN