


MASS SPECTROMETRY REPORT

Product Name: hFSH- β -(33-53) (TFA)

A: 2543.13 \pm 0.41

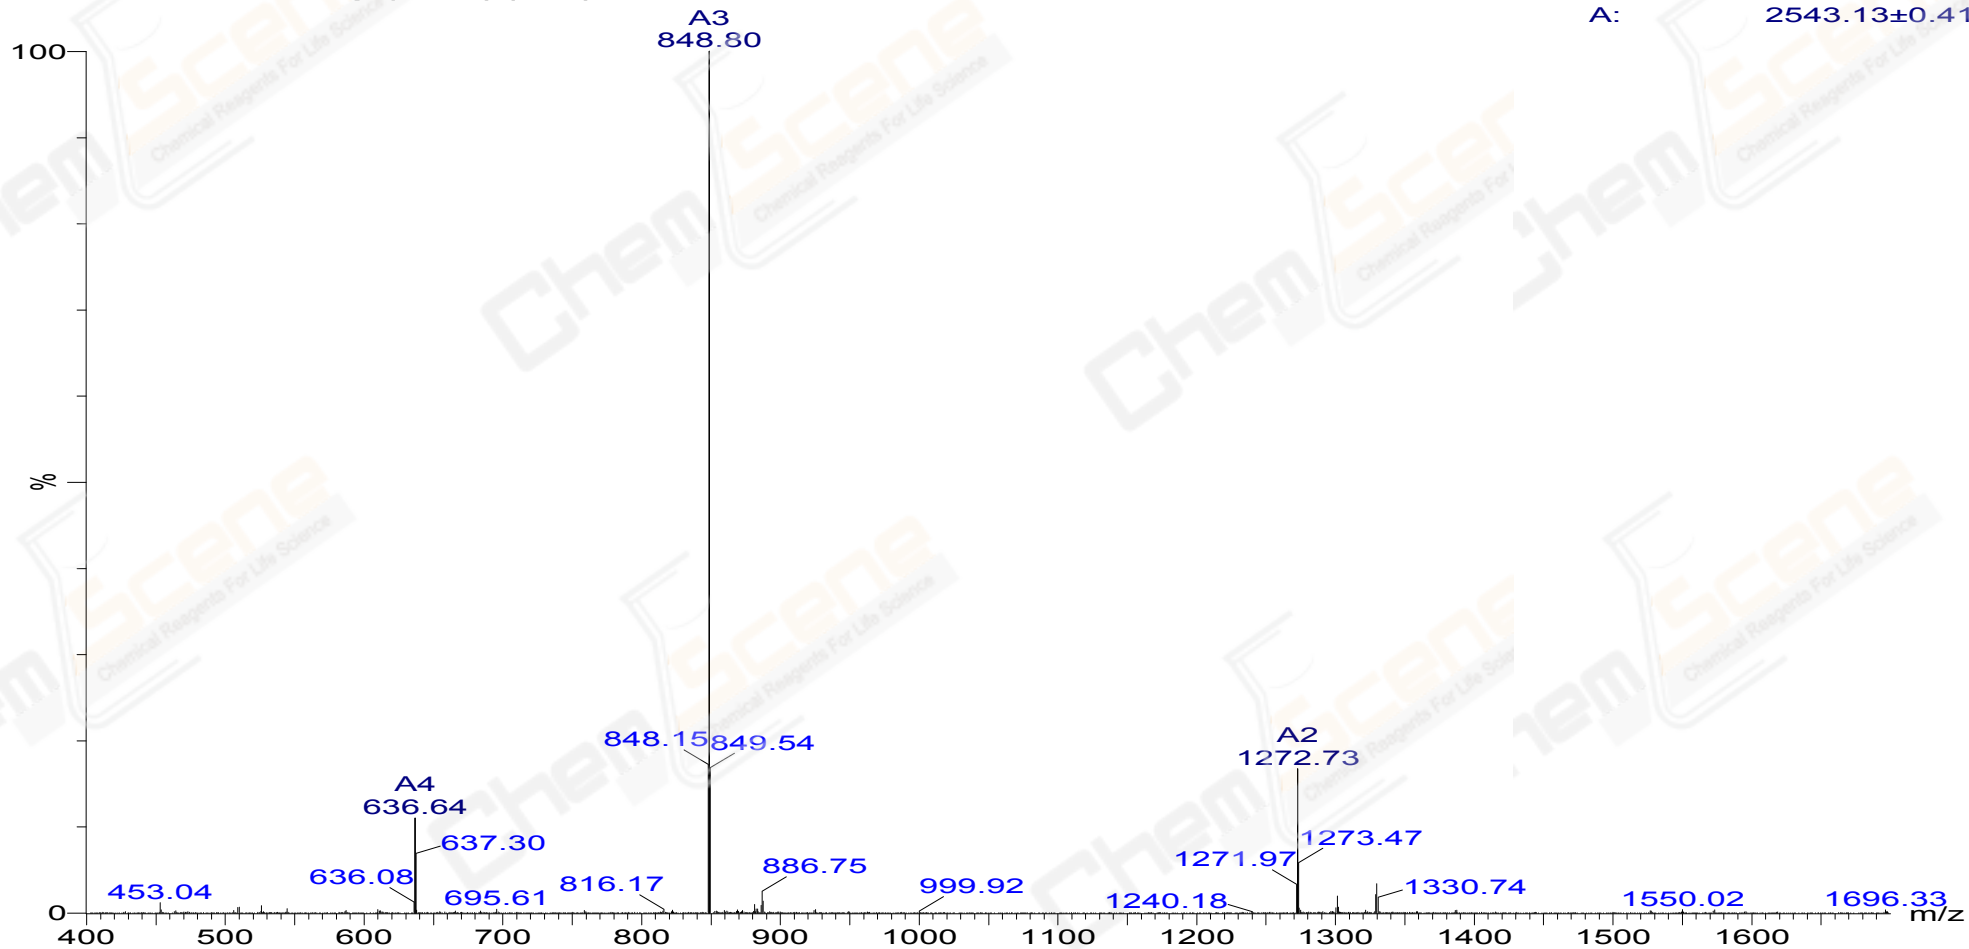

Sample Description

Analyzed date: 2022-03-25
Analyst: SHAO
Sample: 605125
M.W.: 2544.0
Lot. No.:

Instrument

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN